
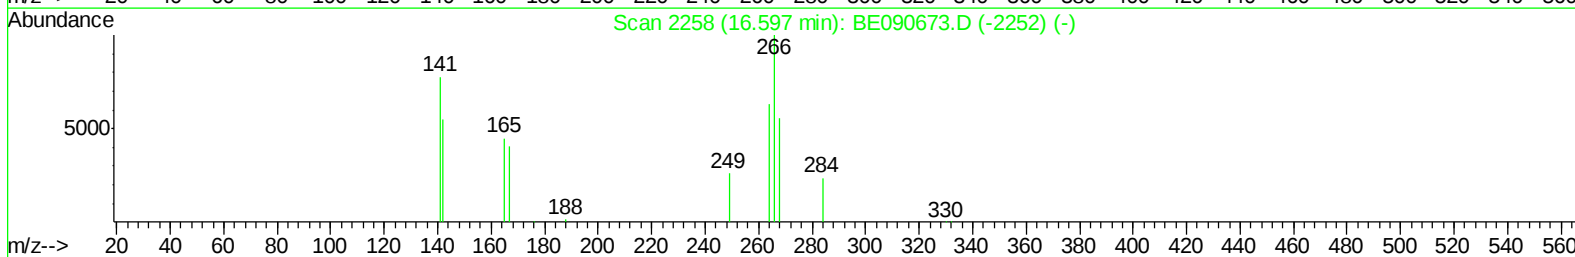
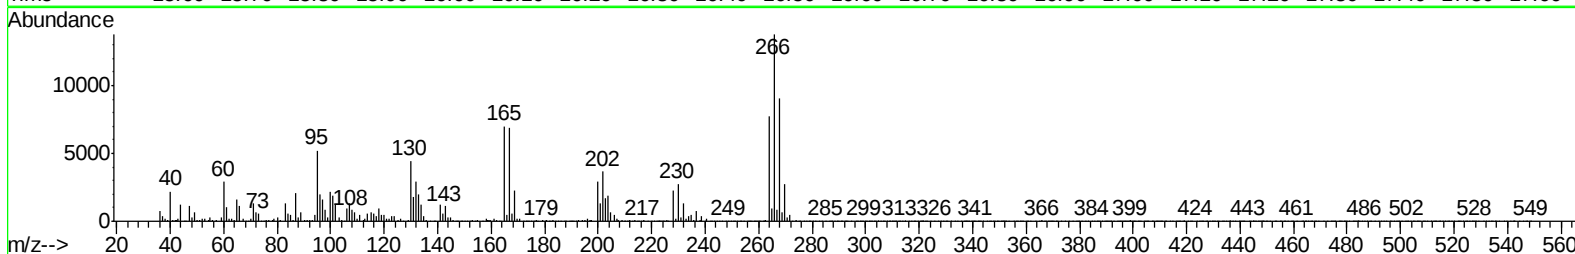


Data Path : Z:\HPCHEM1\BNA E\DATA\BE091015\
Data File : BE090771.D
Acq On : 10 Sep 2015 21:09
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 04:04:13 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 11:40:50 2015
Response via : Initial Calibration

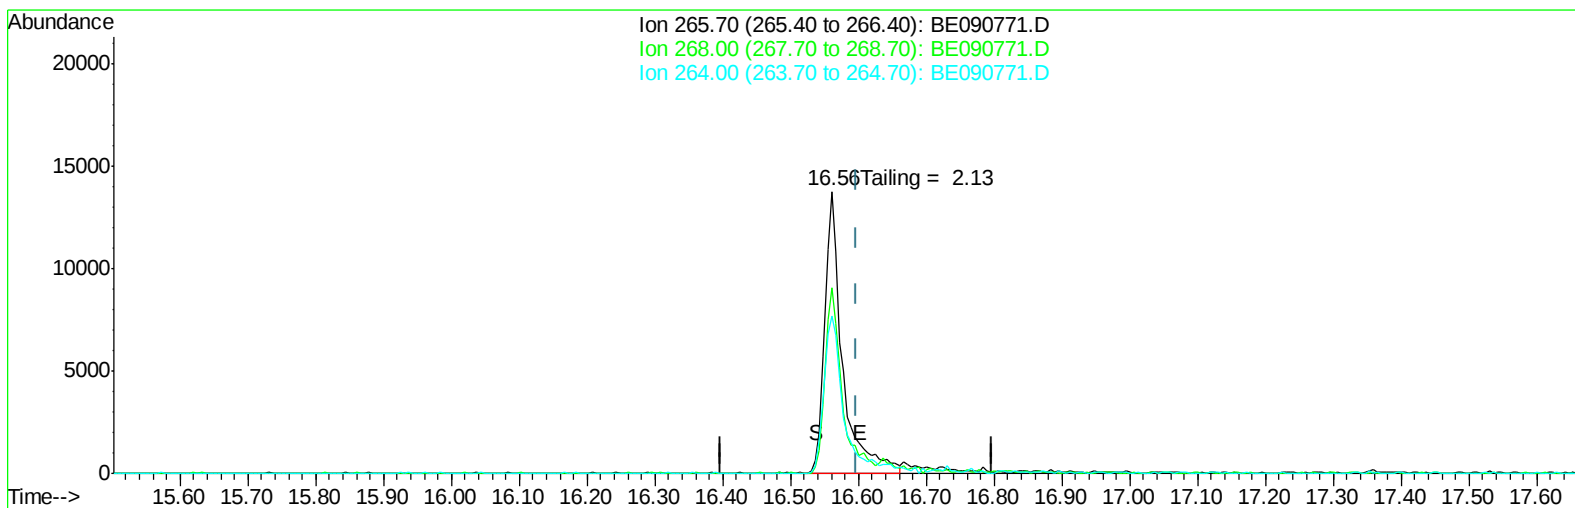

TIC: BE090771.D

(21) Pentachlorophenol

16.560min (-0.037) 56709.34ng m

response 25059

Ion	Exp%	Act%
265.70	100	100
268.00	62.00	65.78
264.00	67.40	55.86
0.00	0.00	0.00