


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091015\
Data File : BE090756.D
Acq On : 10 Sep 2015 10:30
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 02 11:40:50 2015

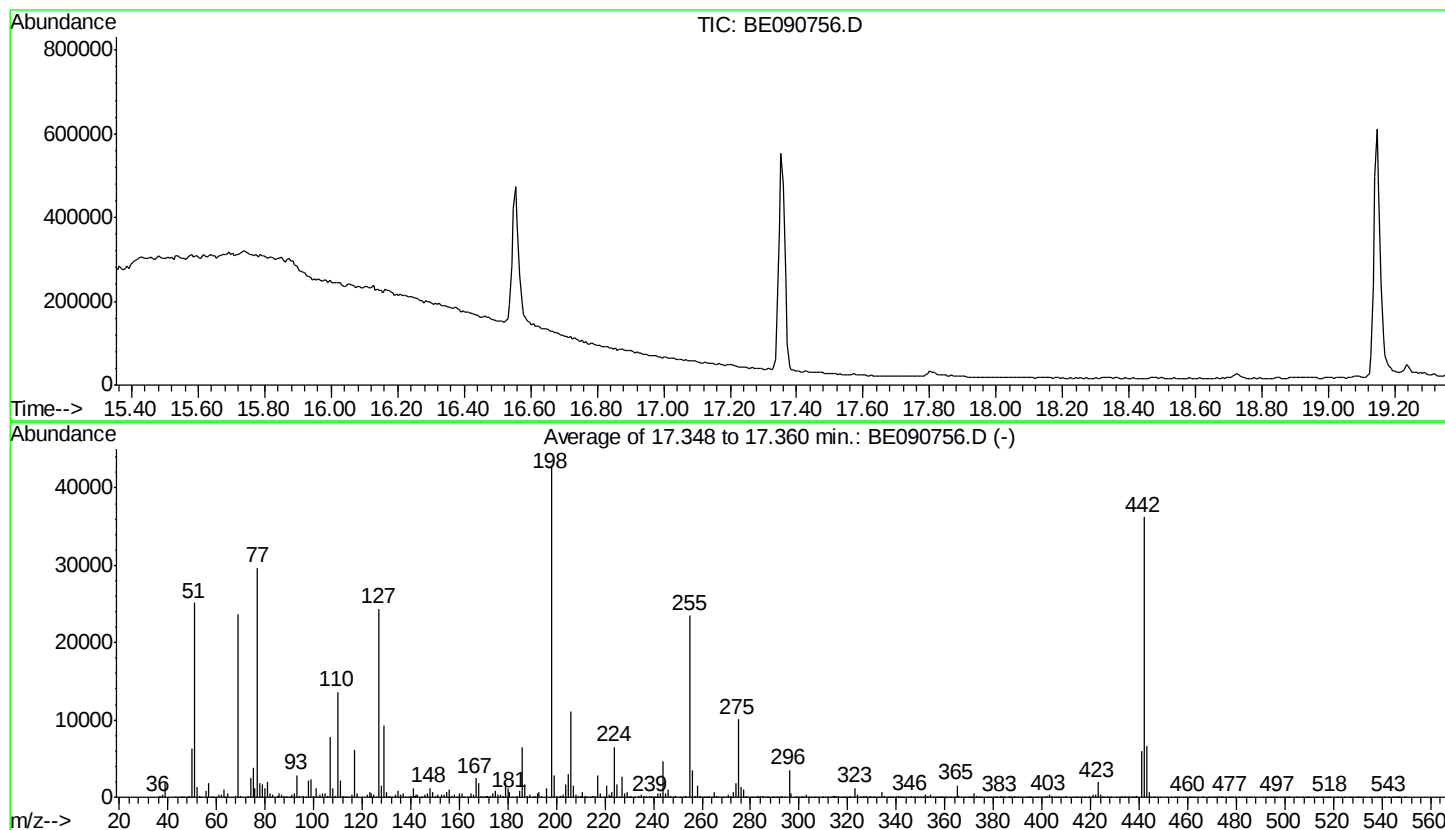

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.6	25149	PASS
68	69	0.00	2	0.8	194	PASS
69	198	0.00	100	55.2	23686	PASS
70	69	0.00	2	0.8	199	PASS
127	198	10	80	56.8	24375	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42896	PASS
199	198	5	9	6.5	2769	PASS
275	198	10	60	23.5	10090	PASS
365	198	1	100	3.5	1503	PASS
441	442	0.01	24	16.4	5938	PASS
442	198	50	100	84.4	36221	PASS
443	442	15	24	18.3	6620	PASS