


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091015\
Data File : BE090771.D
Acq On : 10 Sep 2015 21:09
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 02 11:40:50 2015

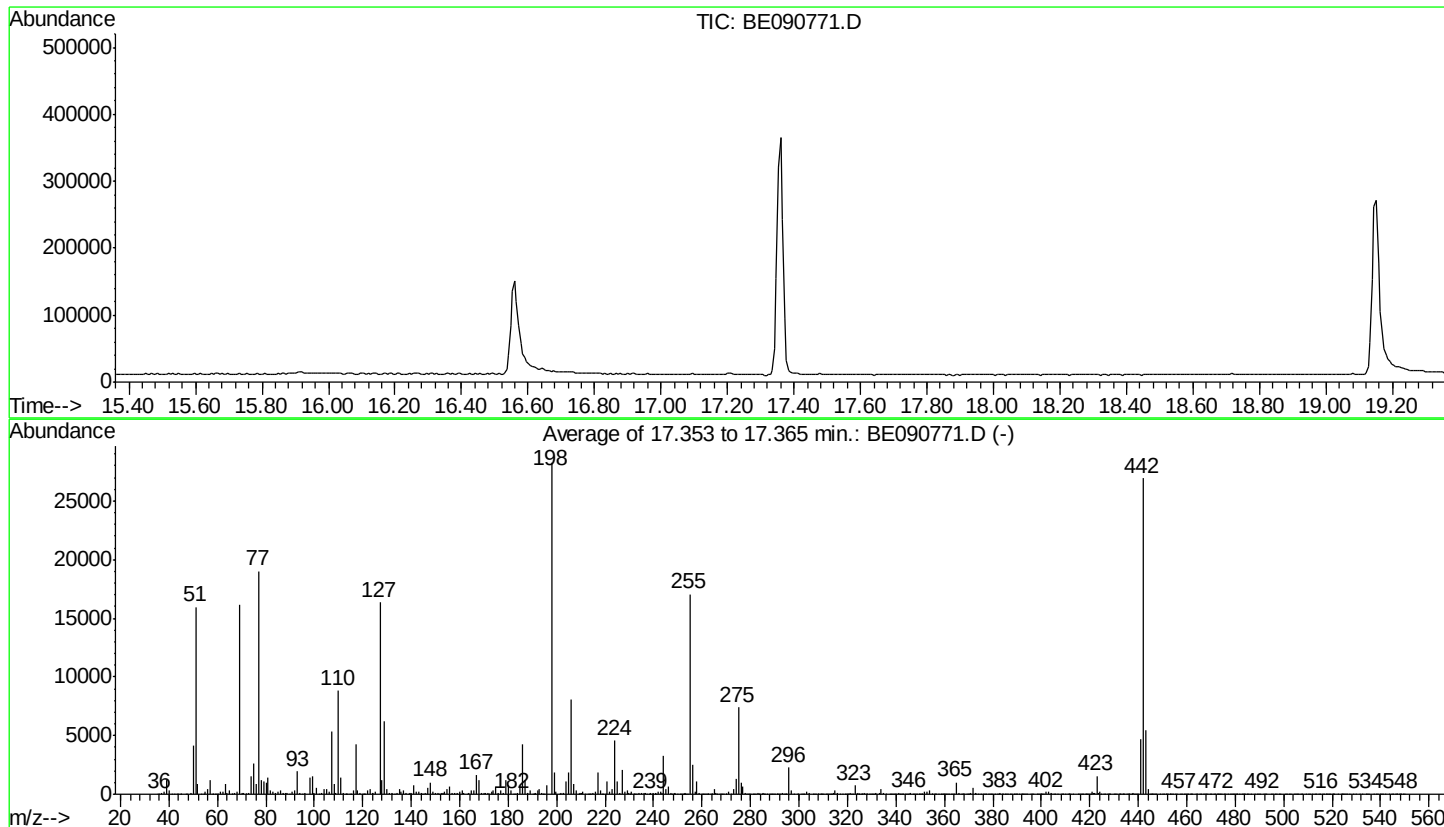

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.4	15933	PASS
68	69	0.00	2	1.6	252	PASS
69	198	0.00	100	57.0	16115	PASS
70	69	0.00	2	0.5	84	PASS
127	198	10	80	57.7	16319	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28266	PASS
199	198	5	9	6.5	1831	PASS
275	198	10	60	26.2	7394	PASS
365	198	1	100	3.6	1012	PASS
441	442	0.01	24	17.5	4719	PASS
442	198	50	100	95.3	26936	PASS
443	442	15	24	20.2	5428	PASS