


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091115\
 Data File : BE090782.D
 Acq On : 11 Sep 2015 11:16
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 02 11:40:50 2015

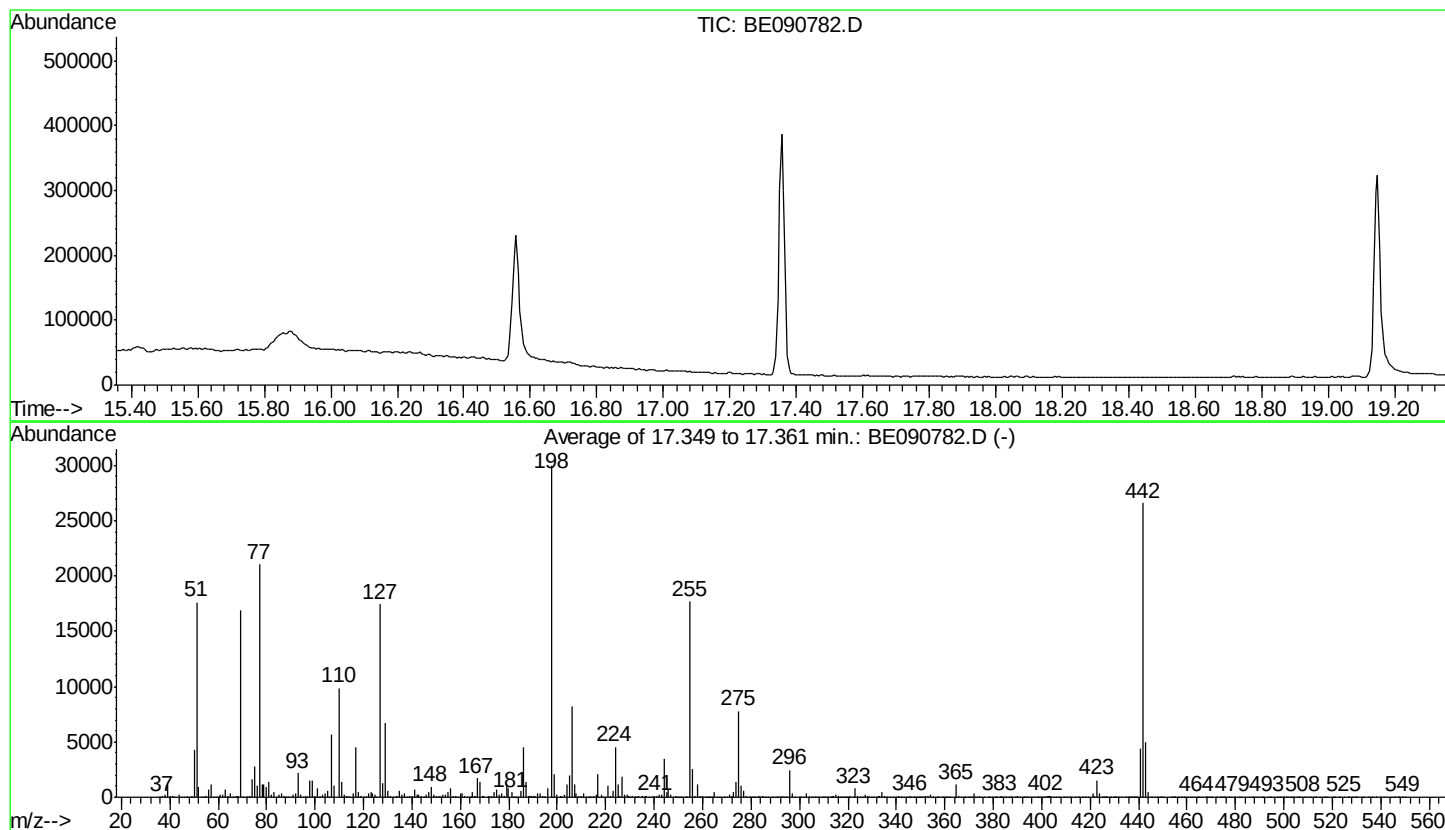

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.8	17629	PASS
68	69	0.00	2	0.7	120	PASS
69	198	0.00	100	56.2	16861	PASS
70	69	0.00	2	0.3	50	PASS
127	198	10	80	58.2	17444	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29976	PASS
199	198	5	9	6.9	2056	PASS
275	198	10	60	25.9	7774	PASS
365	198	1	100	3.7	1105	PASS
441	442	0.01	24	16.7	4438	PASS
442	198	50	100	88.7	26578	PASS
443	442	15	24	18.8	5007	PASS