
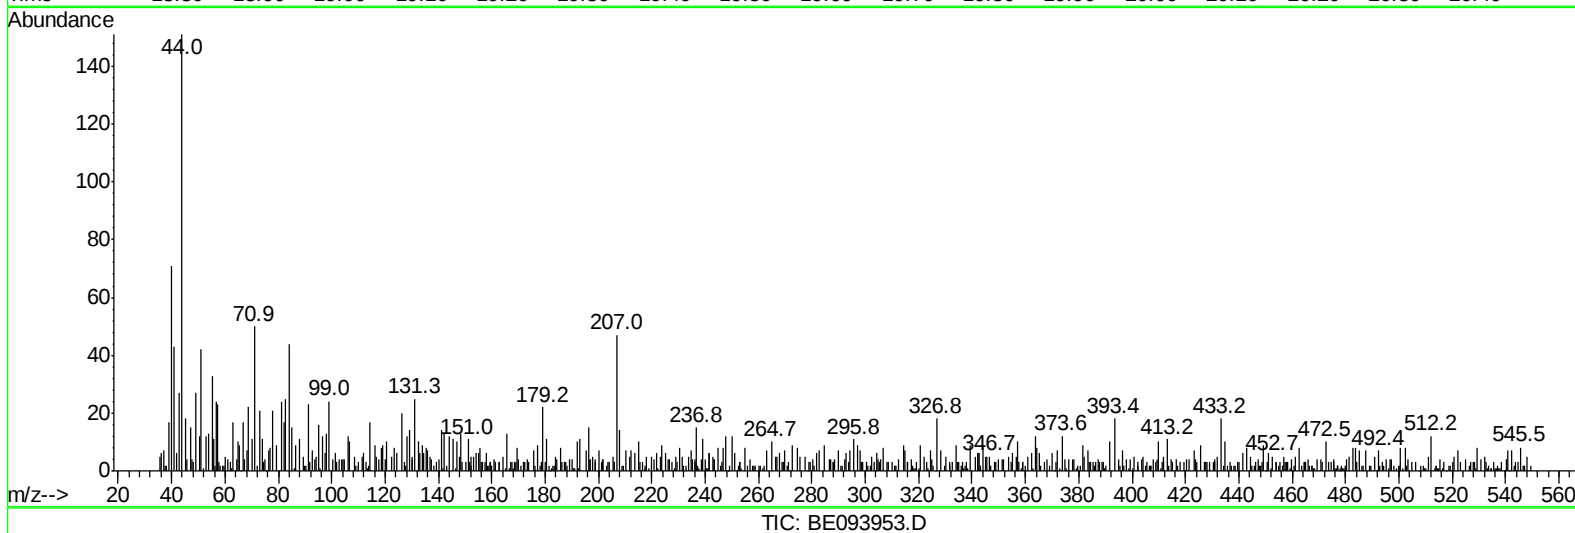


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE091117\
Data File : BE093953.D
Acq On : 11 Sep 2017 9:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 09:00:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

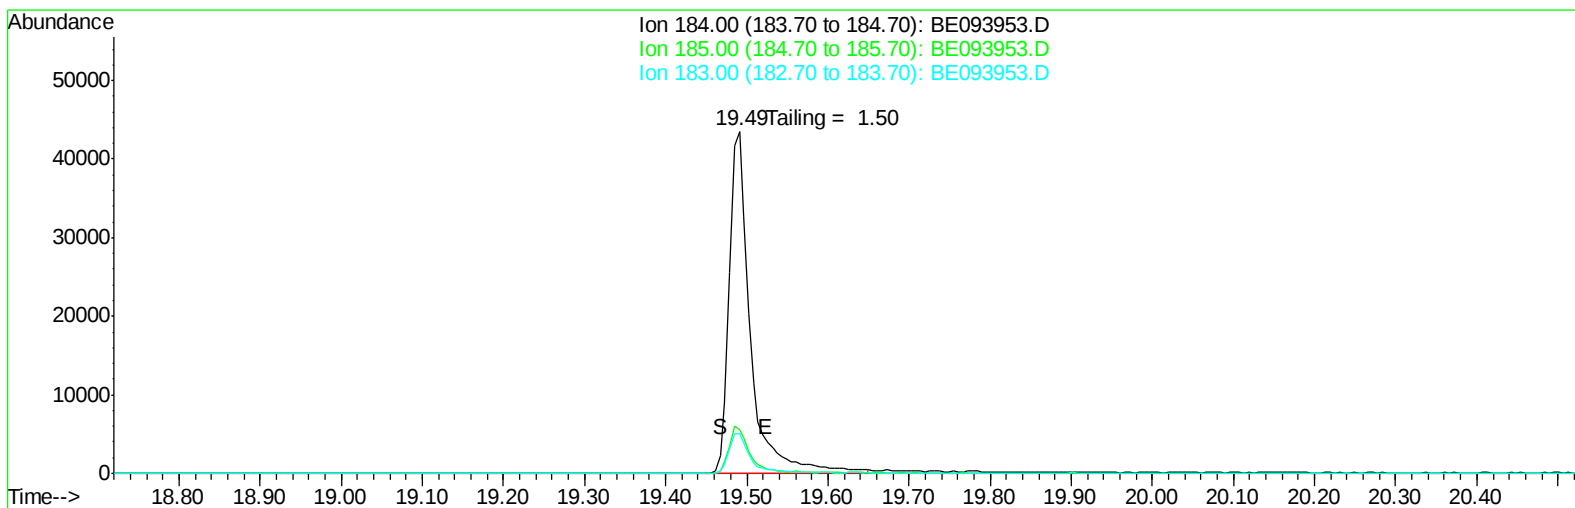

TIC: BE093953.D

(76) Benzidine



12.475min (-0.046) 4.67ng

response 6

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	88.89#
183.00	12.20	44.44#
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE091117\
Data File : BE093953.D
Acq On : 11 Sep 2017 9:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 09:00:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

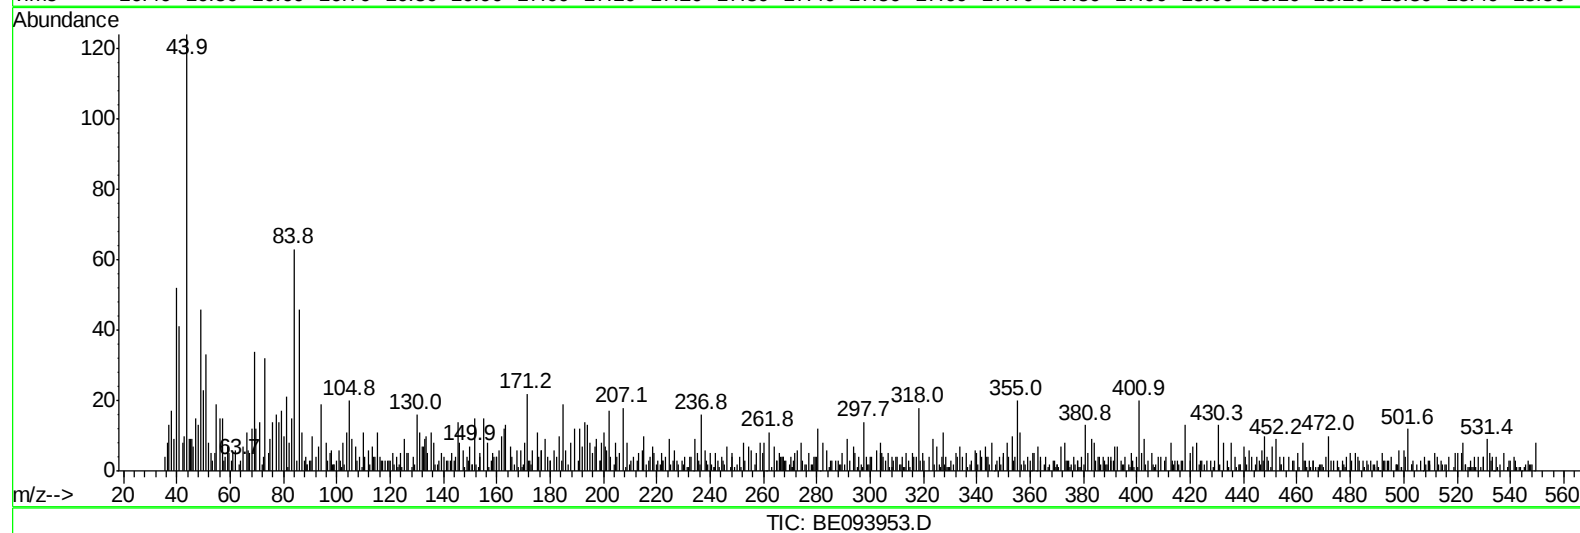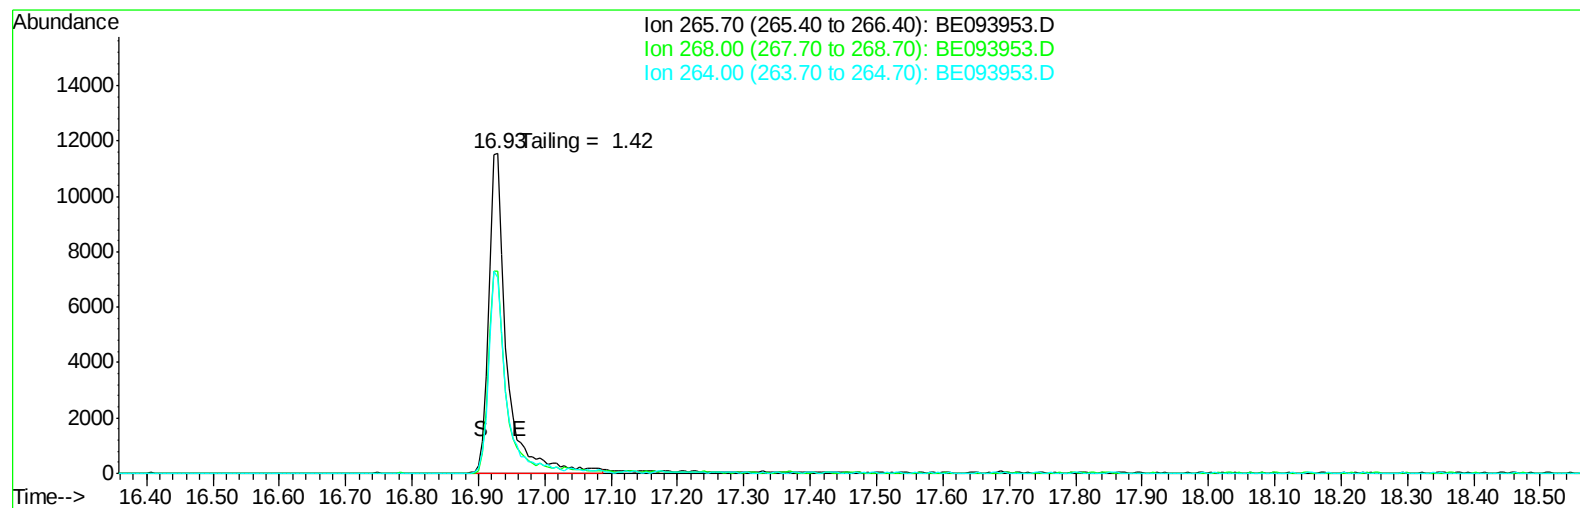

(69) Pentachlorophenol (C)

10.942min (-0.055) 92.66ng

response 4

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.67
264.00	64.60	111.11#
0.00	0.00	0.00