
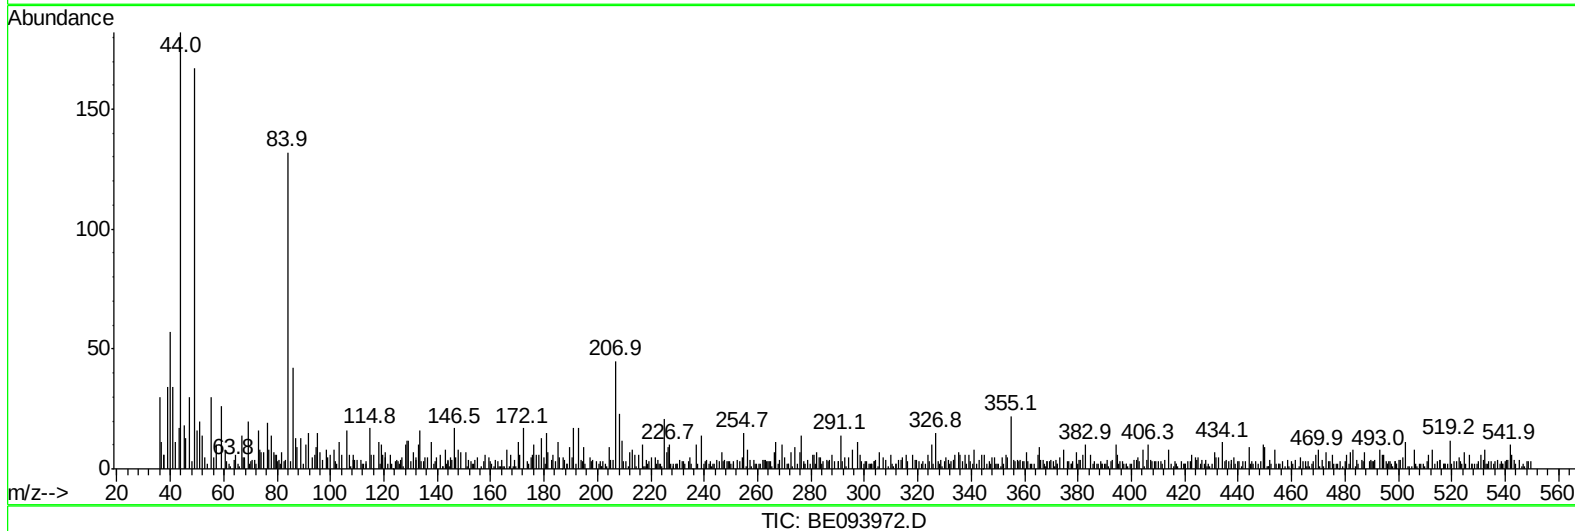


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE091117\  
Data File : BE093972.D  
Acq On : 11 Sep 2017 20:52  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 09:02:04 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 12 02:14:50 2017  
Response via : Initial Calibration

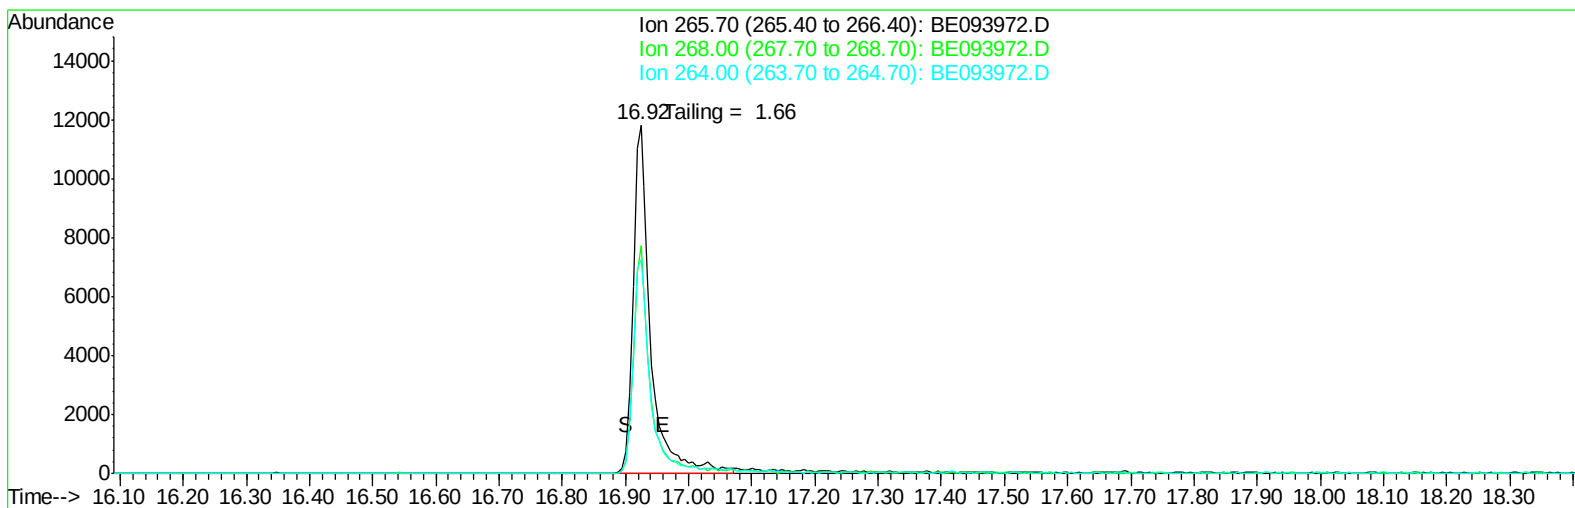

(69) Pentachlorophenol (C)



10.843min (-0.154) 119.73ng

response 10

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 75.00 |
| 264.00 | 64.60 | 75.00 |
| 0.00   | 0.00  | 0.00  |

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE091117\  
Data File : BE093972.D  
Acq On : 11 Sep 2017 20:52  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 09:02:04 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 12 02:14:50 2017  
Response via : Initial Calibration

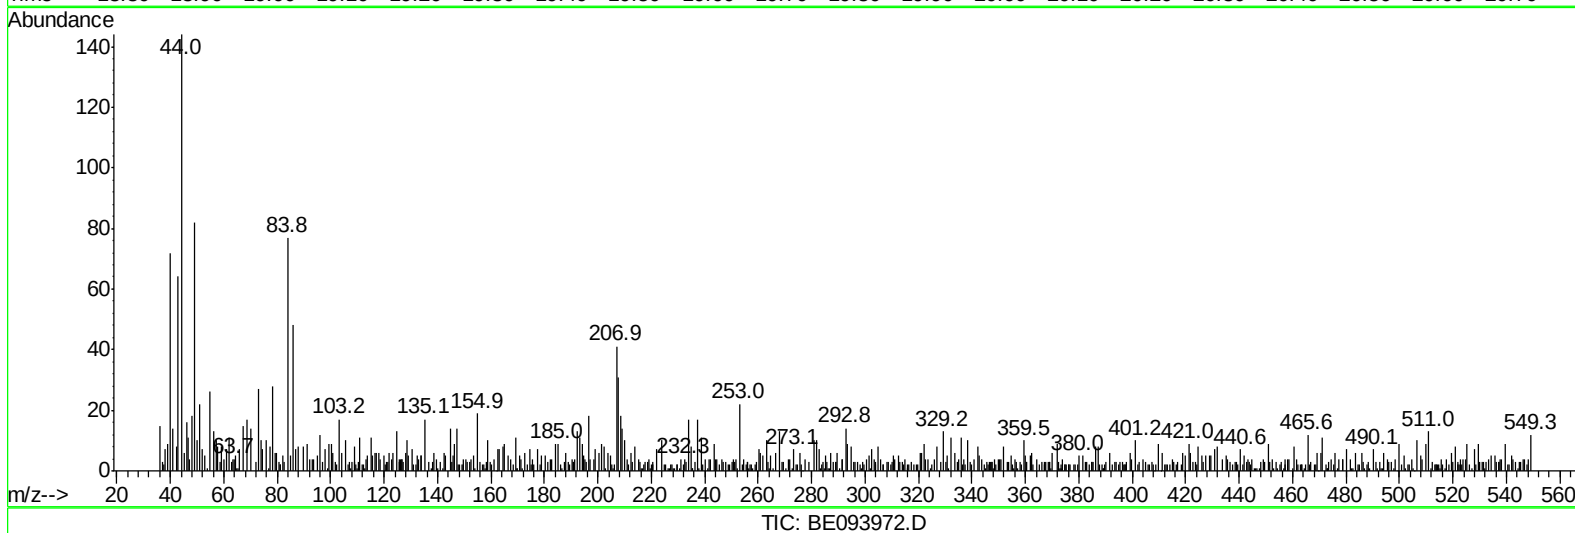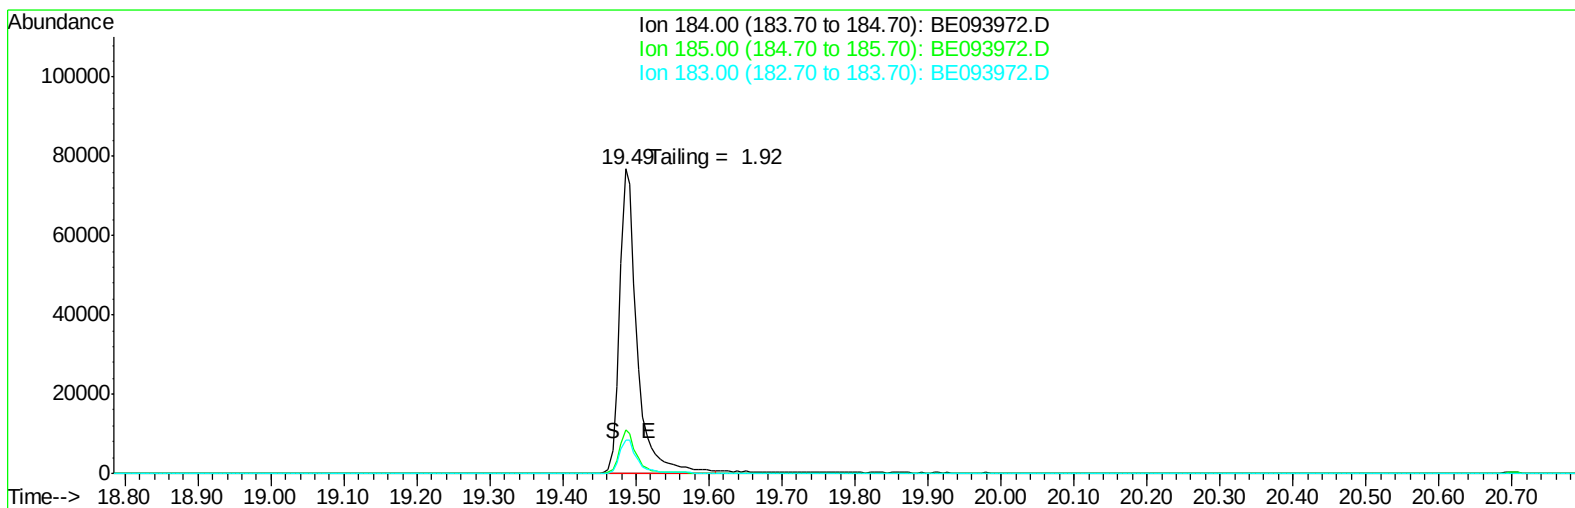

(76) Benzidine

12.582min (+0.061) 13.90ng

response 8

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 184.00 | 100   | 100     |
| 185.00 | 19.40 | 100.00# |
| 183.00 | 12.20 | 44.44#  |
| 0.00   | 0.00  | 0.00    |