

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091117\
 Data File : BE093975.D
 Acq On : 11 Sep 2017 22:42
 Operator : SJ/JU
 Sample : I5147-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 KY038PS033-170906

Quant Time: Sep 12 08:31:51 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 05 13:34:56 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	2531	0.40	ng	0.00
7) Naphthalene-d8	10.71	136	12409	0.40	ng	0.00
13) Acenaphthene-d10	14.53	164	7504	0.40	ng	0.00
19) Phenanthrene-d10	17.24	188	16448	0.40	ng	-0.03
27) Chrysene-d12	21.42	240	18108	0.40	ng	-0.01
34) Perylene-d12	23.93	264	14210	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.53	112	996	0.12	ng	0.00
5) Phenol-d6	7.11	99	867	0.07	ng	0.00
8) Nitrobenzene-d5	9.08	82	3177	0.30	ng	0.00
11) 2-Methylnaphthalene-d10	12.29	152	5766	0.29	ng	0.00
14) 2,4,6-Tribromophenol	16.03	330	479	0.21	ng	0.00
15) 2-Fluorobiphenyl	13.15	172	8236	0.28	ng	-0.01
25) Fluoranthene-d10	19.27	212	63276	0.26	ng	0.00
29) Terphenyl-d14	19.86	244	12193	0.37	ng	-0.01
Target Compounds						Qvalue
32) Bis(2-ethylhexyl)phthalate	21.29	149	14831	0.110	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091117\
Data File : BE093975.D
Acq On : 11 Sep 2017 22:42
Operator : SJ/JU
Sample : I5147-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
KY038PS033-170906

Quant Time: Sep 12 08:31:51 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 05 13:34:56 2017
Response via : Initial Calibration

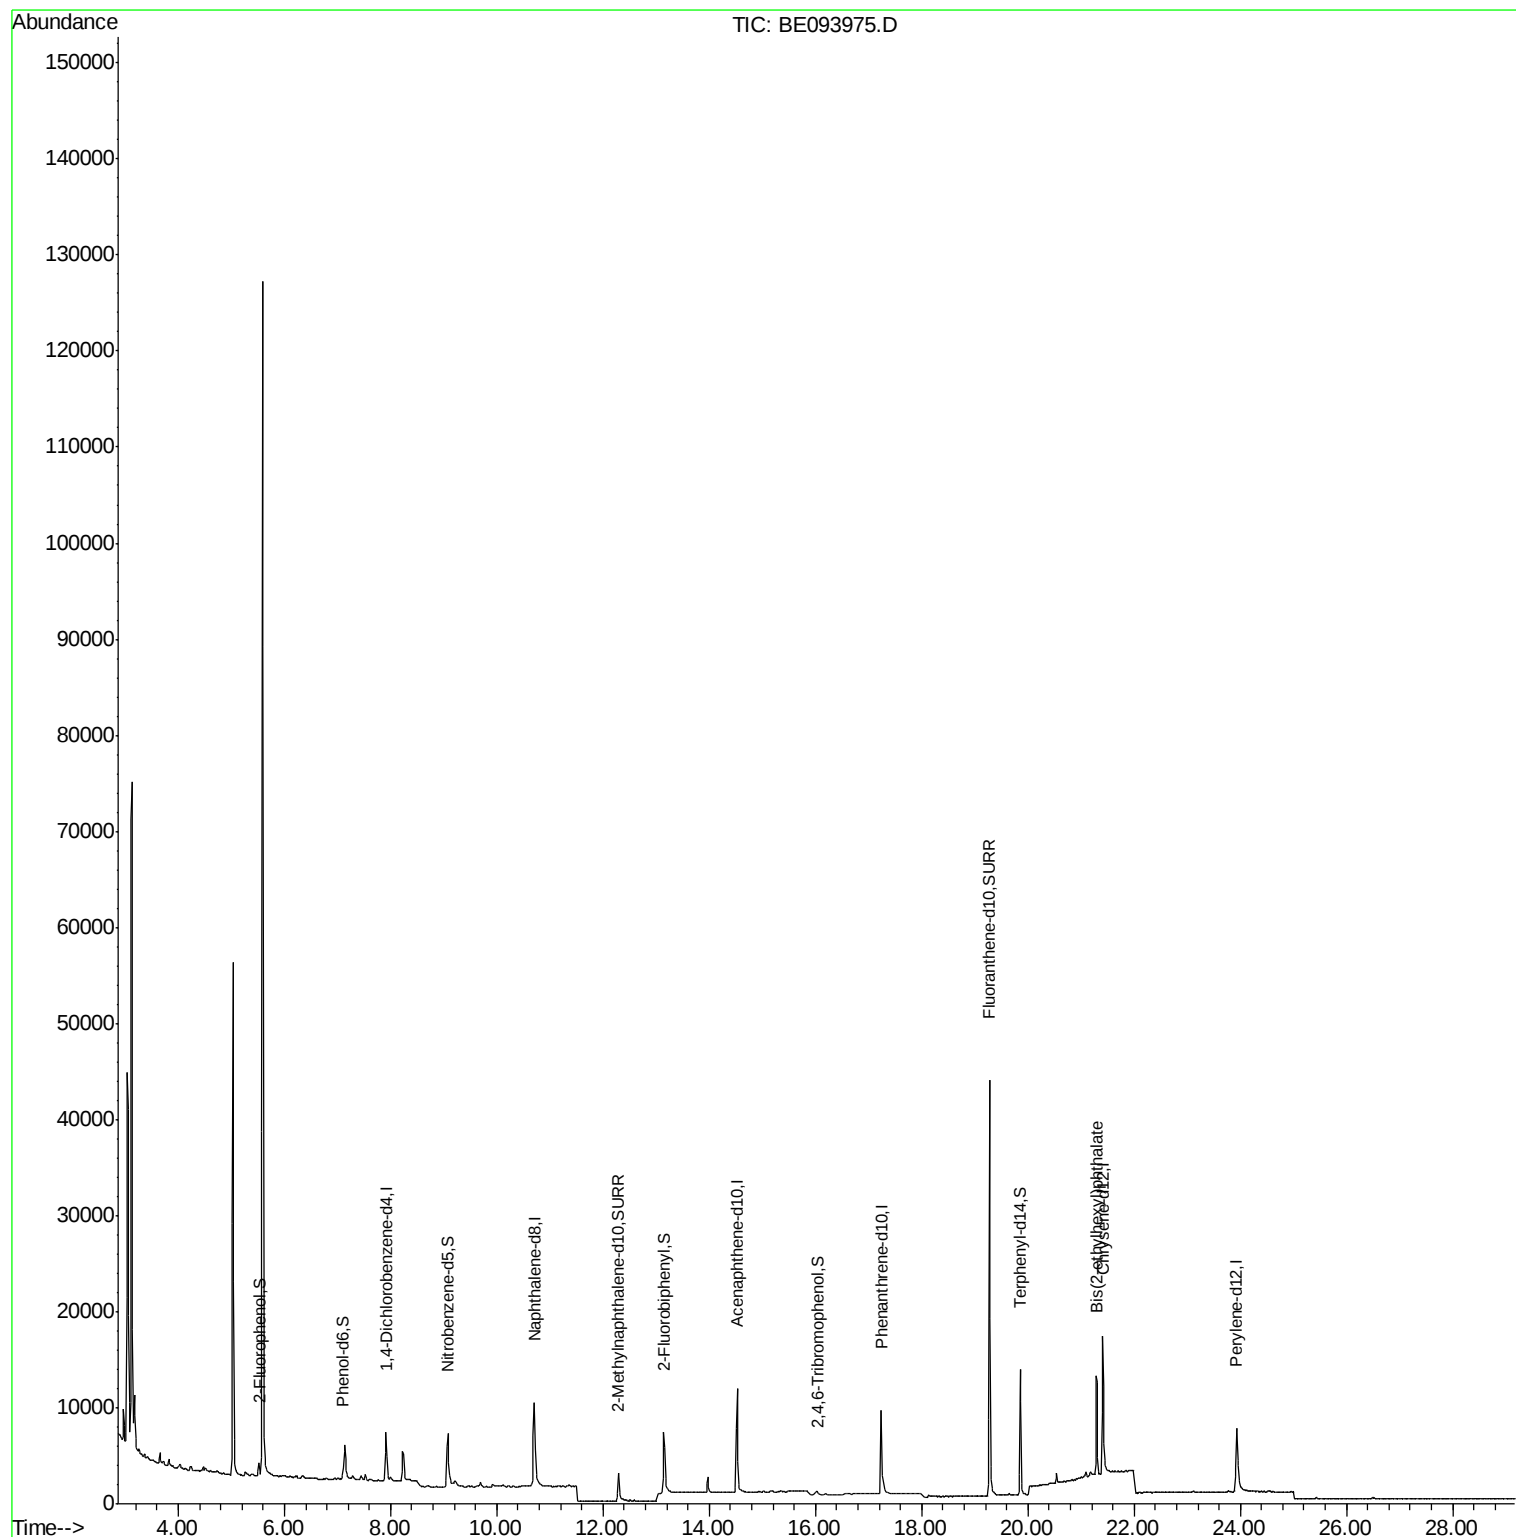

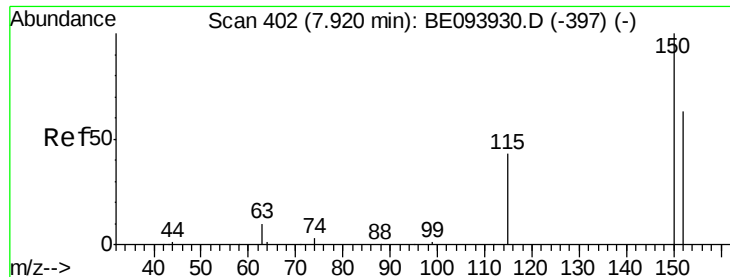

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.92 min Scan# 402

Delta R.T. -0.00 min

Lab File: BE093975.D

Acq: 11 Sep 2017 22:42

Instrument :

BNA_E

ClientSampleId :

KY038PS033-170906


Tgt Ion:152 Resp: 2531

Ion Ratio Lower Upper

152 100

150 155.4 121.8 182.6




115 67.4 52.6 79.0

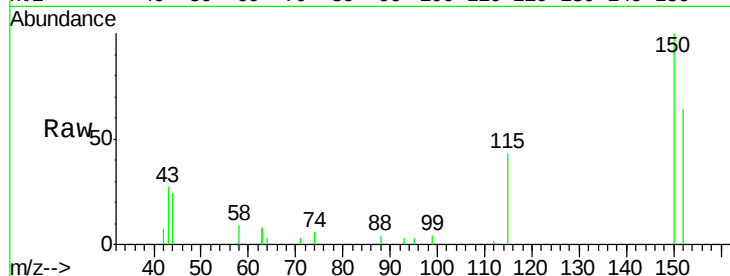

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

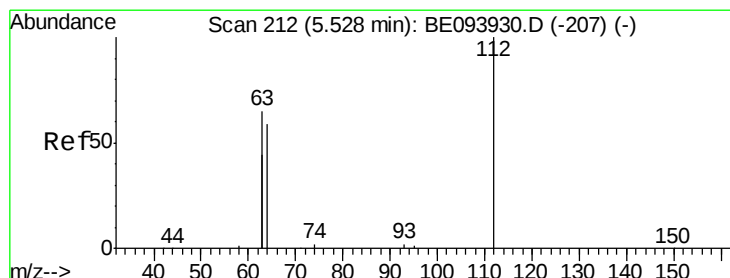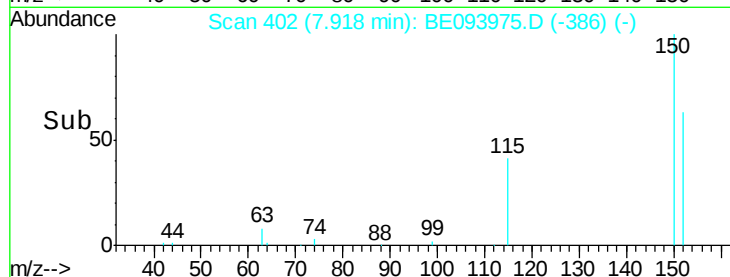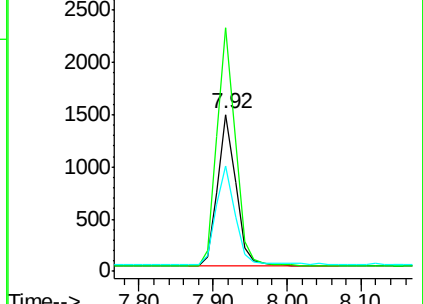

#4

2-Fluorophenol

Concen: 0.122 ng

RT: 5.53 min Scan# 212

Delta R.T. -0.00 min

Lab File: BE093975.D

Acq: 11 Sep 2017 22:42


Tgt Ion:112 Resp: 996

Ion Ratio Lower Upper

112 100

64 68.0 57.7 86.5



63 137.9 116.0 174.0

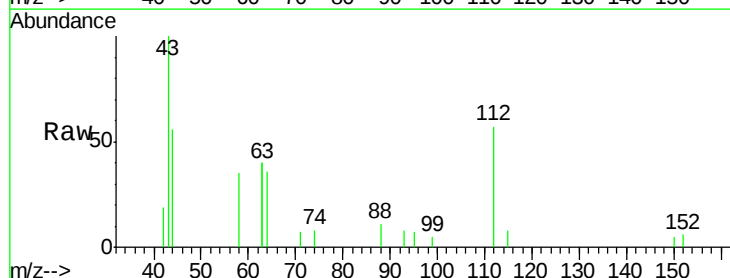


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

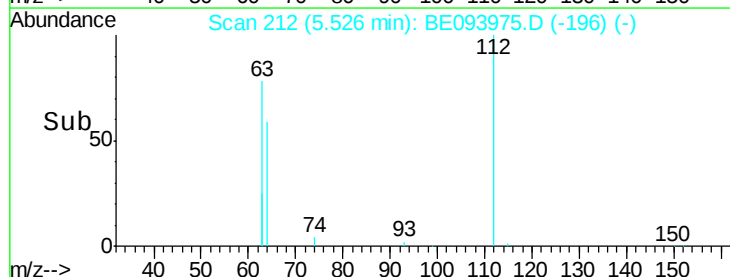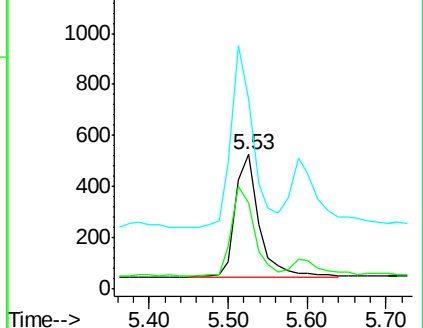

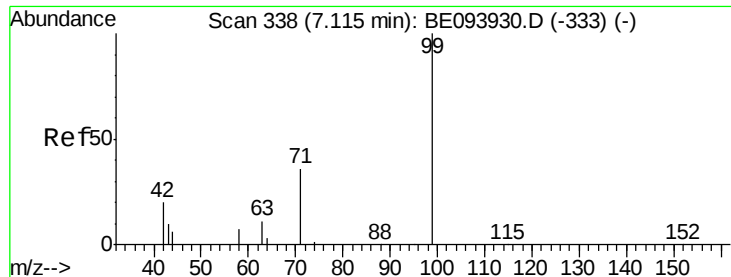

#5

Phenol-d6

Concen: 0.071 ng

RT: 7.11 min Scan# 338

Delta R.T. -0.00 min

Lab File: BE093975.D

Acq: 11 Sep 2017 22:42

Instrument :

BNA_E

ClientSampleId :

KY038PS033-170906


Tgt Ion: 99 Resp: 867

Ion Ratio Lower Upper




99 100

42 40.5 17.1 25.7#

71 38.4 26.6 39.8

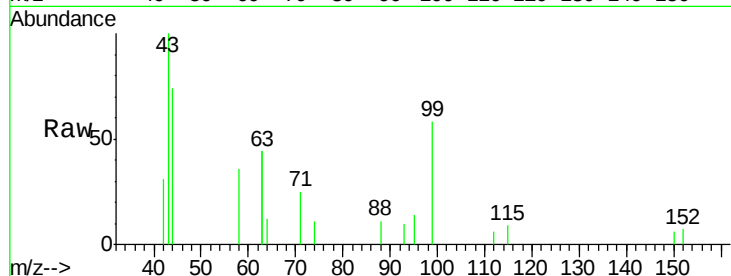

Abundance Ion 99.00 (98.70 to 99.70): BE0
Ion 42.00 (41.70 to 42.70): BE0
Ion 71.00 (70.70 to 71.70): BE0

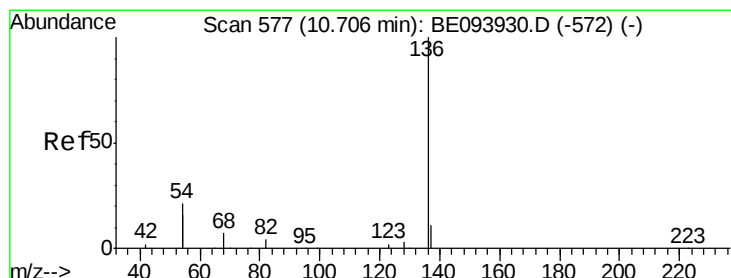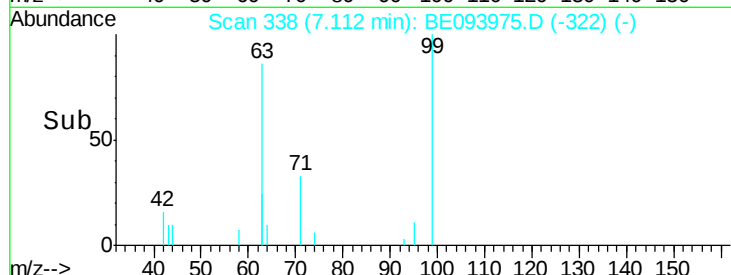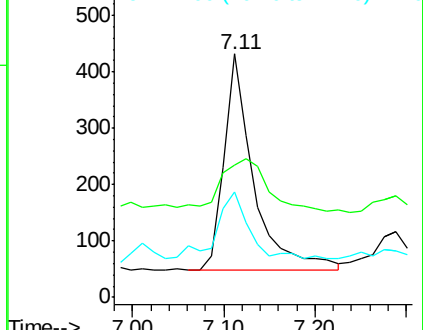

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.71 min Scan# 577

Delta R.T. 0.00 min

Lab File: BE093975.D

Acq: 11 Sep 2017 22:42

Tgt Ion: 136 Resp: 12409


Ion Ratio Lower Upper

136 100



137 11.8 9.2 13.8


54 34.3 21.9 32.9#

68 7.0 4.6 7.0#

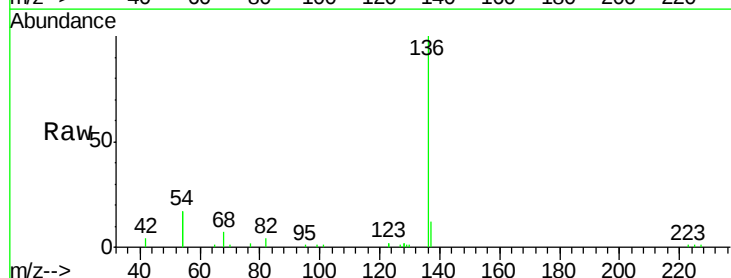

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BE0
Ion 68.00 (67.70 to 68.70): BE0

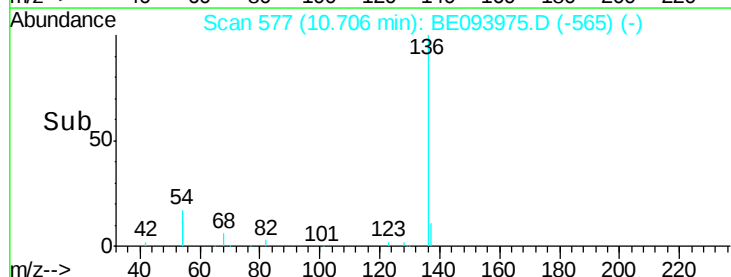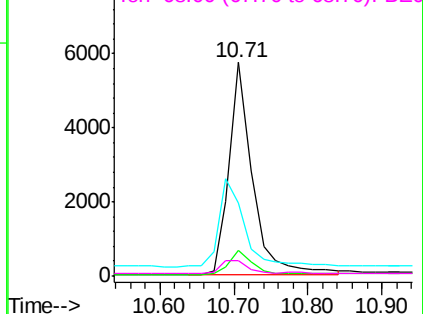

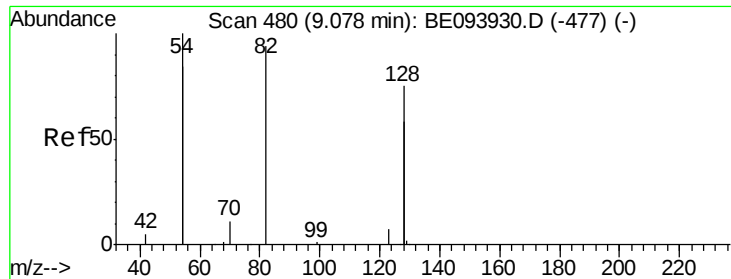

#8

Nitrobenzene-d5

Concen: 0.303 ng

RT: 9.08 min Scan# 480

Delta R.T. 0.00 min

Lab File: BE093975.D

Acq: 11 Sep 2017 22:42

Instrument :

BNA_E

ClientSampleId :

KY038PS033-170906


Tgt Ion: 82 Resp: 3177

Ion Ratio Lower Upper

82 100

128 160.6 91.4 137.0#




54 200.3 197.8 296.8

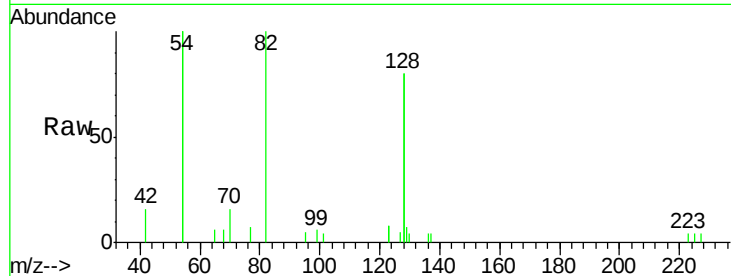

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

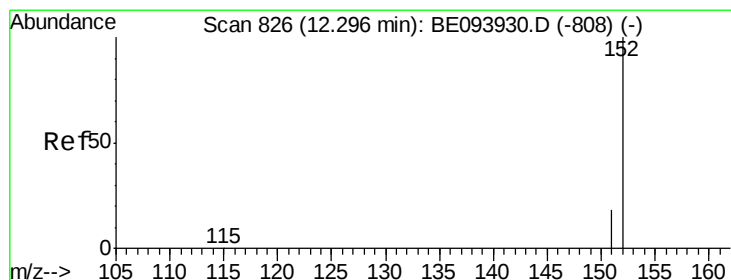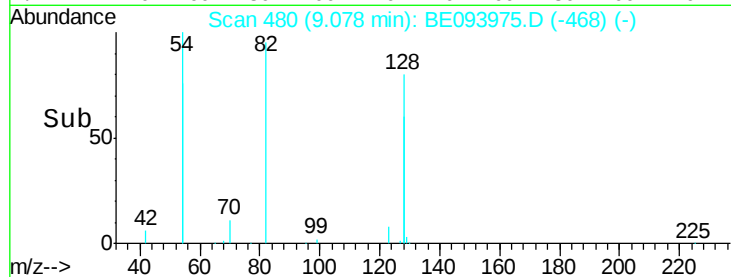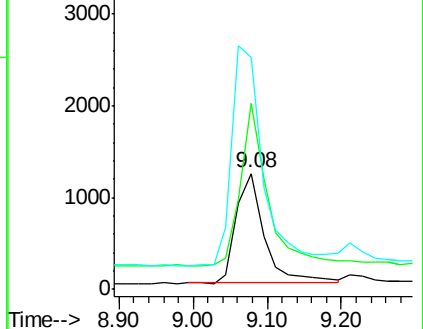

#11

2-Methylnaphthalene-d10

Concen: 0.290 ng

RT: 12.29 min Scan# 825

Delta R.T. -0.00 min

Lab File: BE093975.D


Acq: 11 Sep 2017 22:42

Tgt Ion: 152 Resp: 5766

Ion Ratio Lower Upper



152 100


151 18.8 15.4 23.0

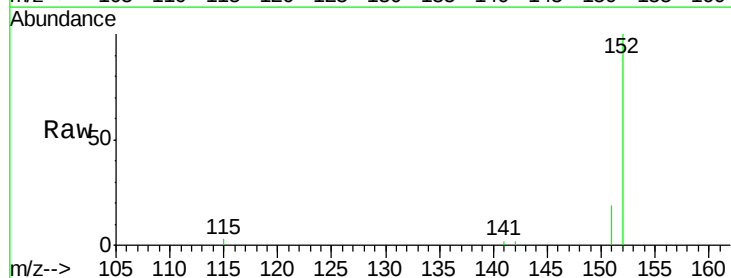

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

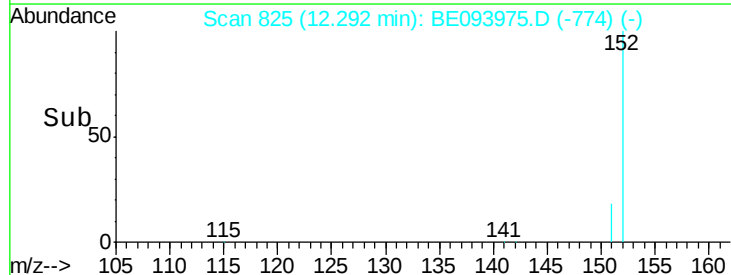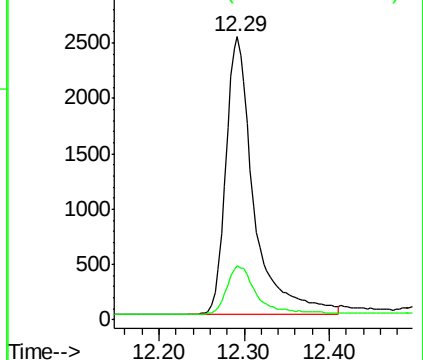

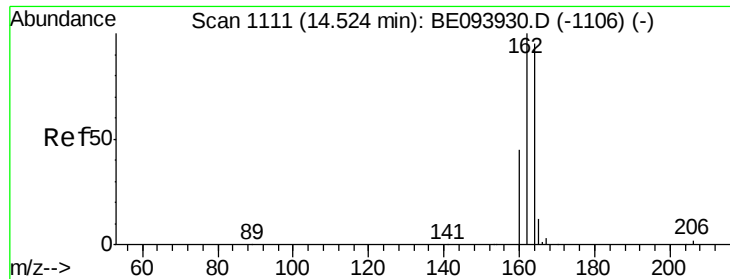

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.53 min Scan# 1112

Delta R.T. 0.00 min

Lab File: BE093975.D

Acq: 11 Sep 2017 22:42

Instrument :

BNA_E

ClientSampleId :

KY038PS033-170906


Tgt Ion:164 Resp: 7504

Ion Ratio Lower Upper

164 100

162 104.3 80.8 121.2




160 47.0 37.0 55.4

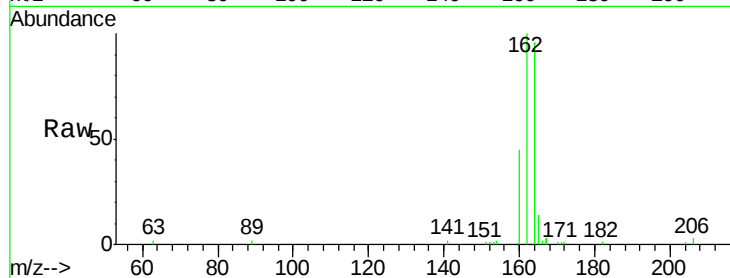

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

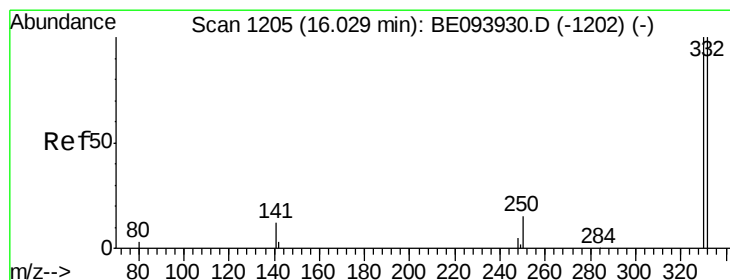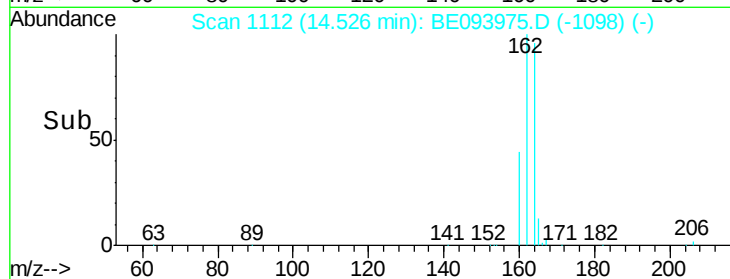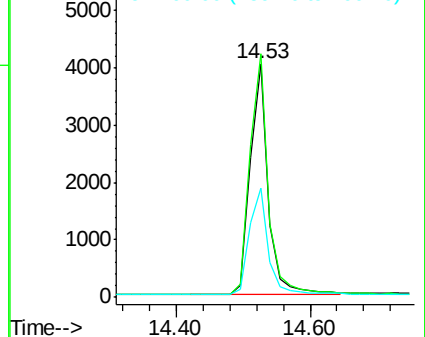

#14

2,4,6-Tribromophenol

Concen: 0.206 ng

RT: 16.03 min Scan# 1206

Delta R.T. 0.00 min

Lab File: BE093975.D

Acq: 11 Sep 2017 22:42


Tgt Ion:330 Resp: 479

Ion Ratio Lower Upper

330 100

332 107.3 76.9 115.3



141 0.0 0.0 0.0

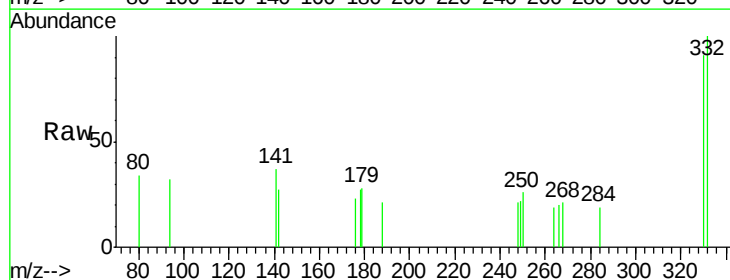


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



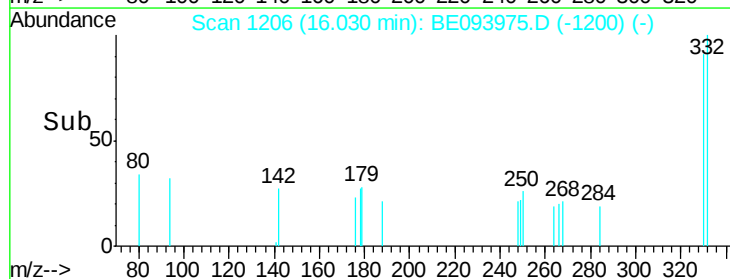
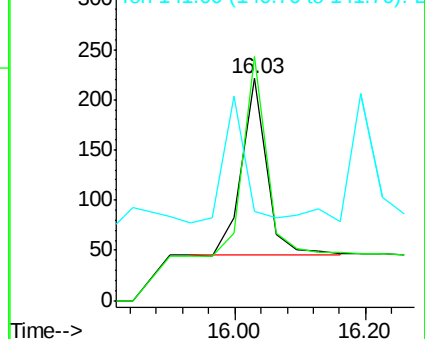


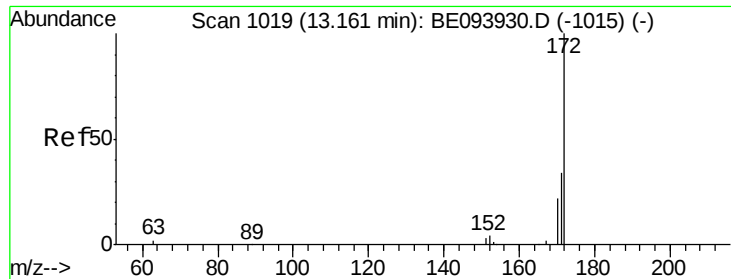

#15
2-Fluorobiphenyl
Concen: 0.278 ng
RT: 13.15 min Scan# 1019
Delta R.T. -0.01 min
Lab File: BE093975.D
Acq: 11 Sep 2017 22:42




Instrument :
BNA_E
ClientSampleId :
KY038PS033-170906


Tgt Ion:172 Resp: 8236
Ion Ratio Lower Upper
172 100
171 36.5 26.9 40.3
170 25.3 17.3 25.9

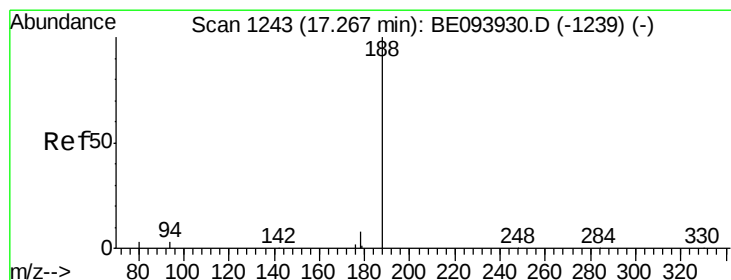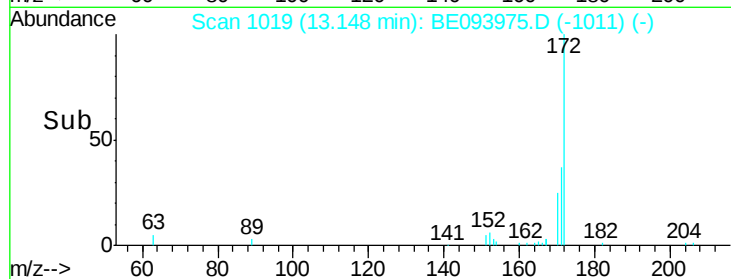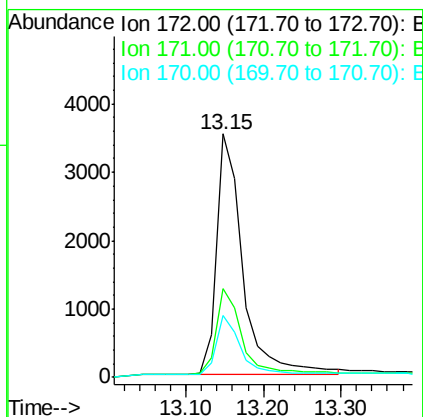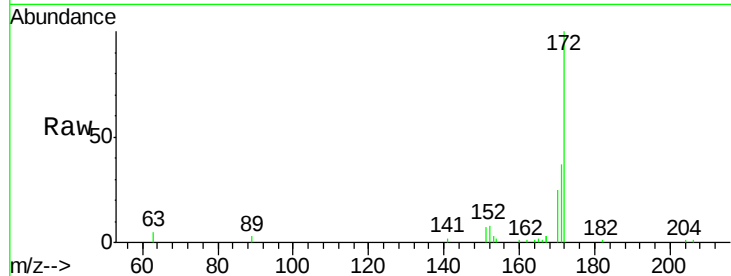

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.24 min Scan# 1243
Delta R.T. -0.03 min
Lab File: BE093975.D
Acq: 11 Sep 2017 22:42

Tgt Ion:188 Resp: 16448
Ion Ratio Lower Upper
188 100
94 18.8 16.1 24.1
80 21.0 18.2 27.2

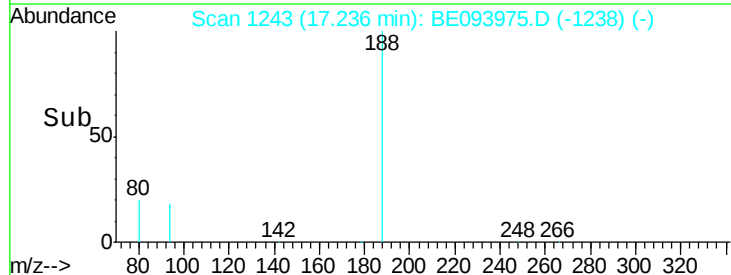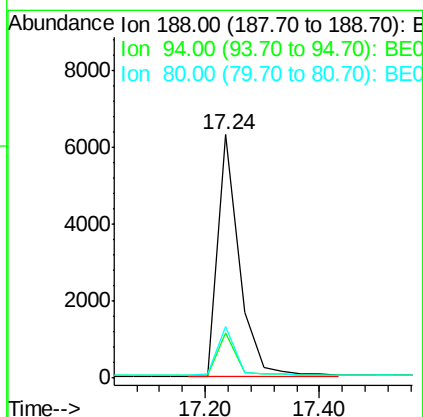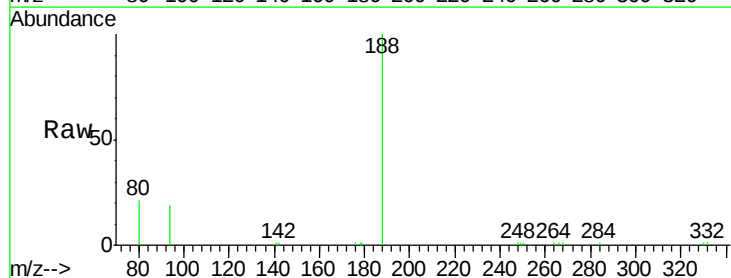

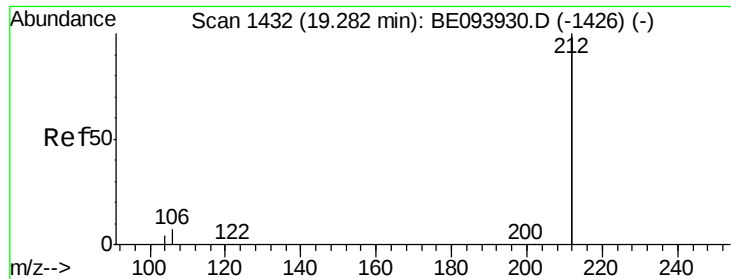

#25

Fluoranthene-d10

Concen: 0.258 ng

RT: 19.27 min Scan# 1432

Delta R.T. -0.01 min

Lab File: BE093975.D

Acq: 11 Sep 2017 22:42

Instrument :

BNA_E

ClientSampleId :

KY038PS033-170906


Tgt Ion:212 Resp: 63276

Ion Ratio Lower Upper

212 100

106 3.4 2.7 4.1




104 2.0 1.6 2.4

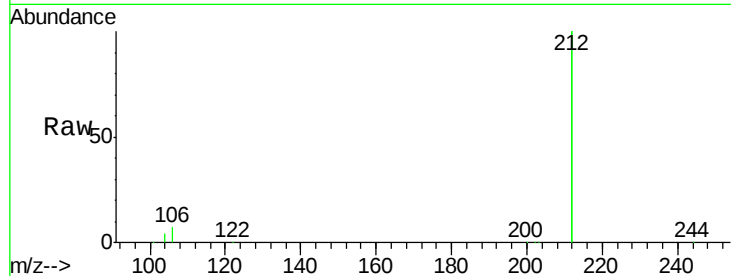

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

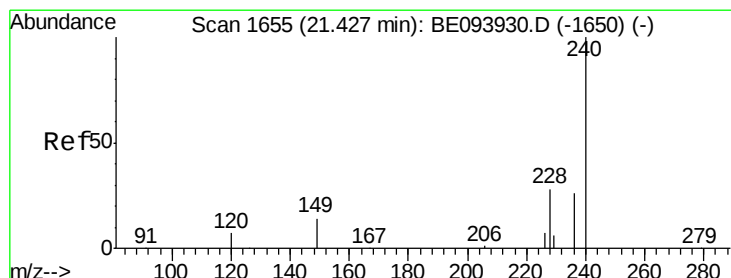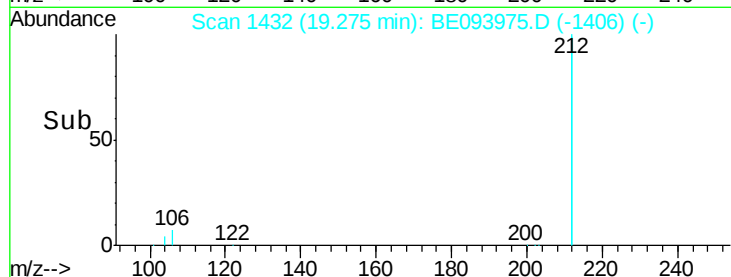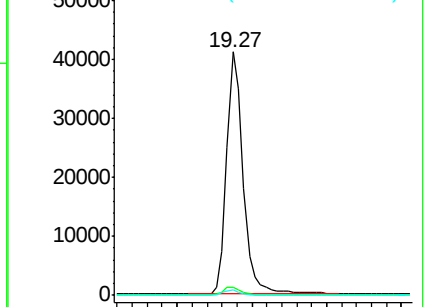

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.42 min Scan# 1655

Delta R.T. -0.01 min

Lab File: BE093975.D

Acq: 11 Sep 2017 22:42


Tgt Ion:240 Resp: 18108

Ion Ratio Lower Upper

240 100

120 11.7 8.7 13.1



236 27.6 21.3 31.9

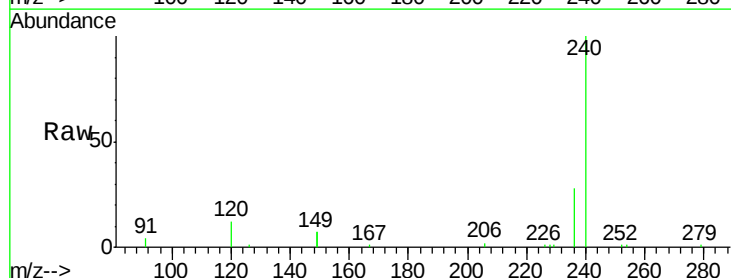


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

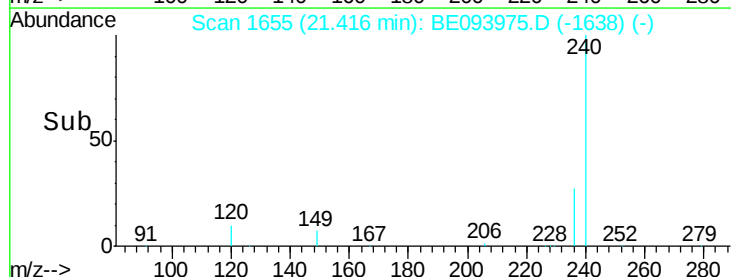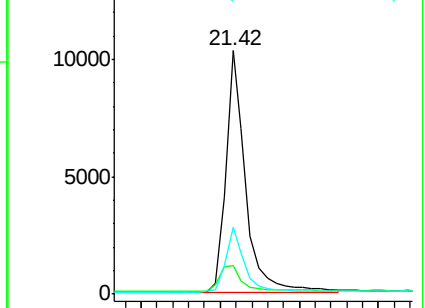

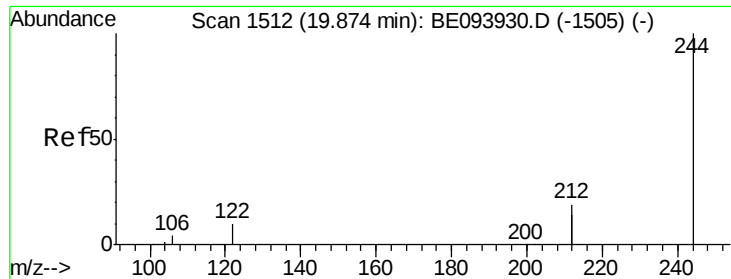

#29

Terphenyl-d14

Concen: 0.366 ng

RT: 19.86 min Scan# 1511

Delta R.T. -0.01 min

Lab File: BE093975.D

Acq: 11 Sep 2017 22:42

Instrument :

BNA_E

ClientSampleId :

KY038PS033-170906


Tgt Ion:244 Resp: 12193

Ion Ratio Lower Upper

244 100

212 33.7 28.3 42.5




122 12.8 9.4 14.0

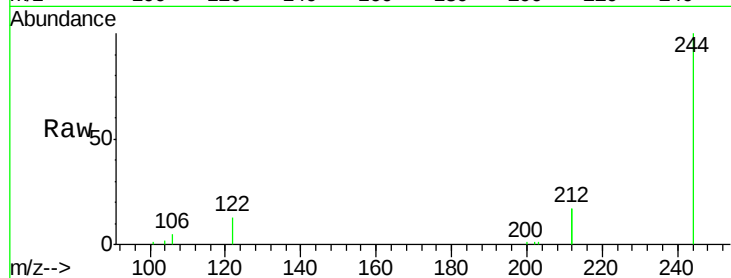

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

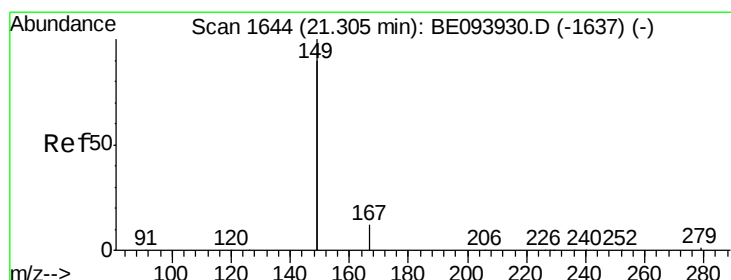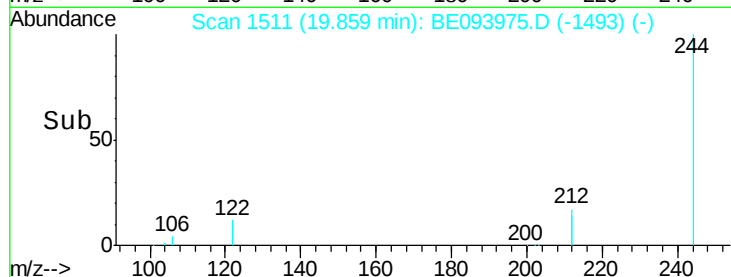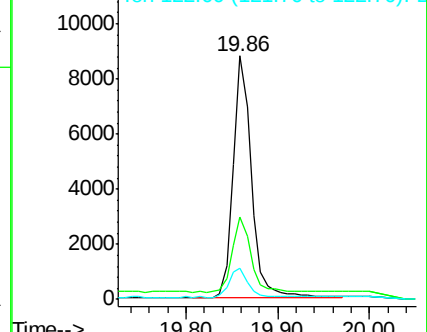

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.110 ng

RT: 21.29 min Scan# 1644

Delta R.T. -0.01 min

Lab File: BE093975.D

Acq: 11 Sep 2017 22:42


Tgt Ion:149 Resp: 14831

Ion Ratio Lower Upper

149 100

167 6.6 5.4 8.0



279 1.0 0.7 1.1



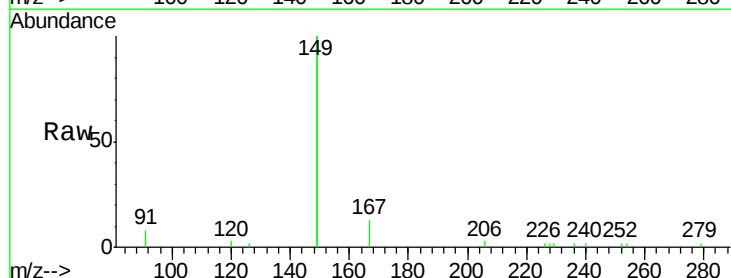


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

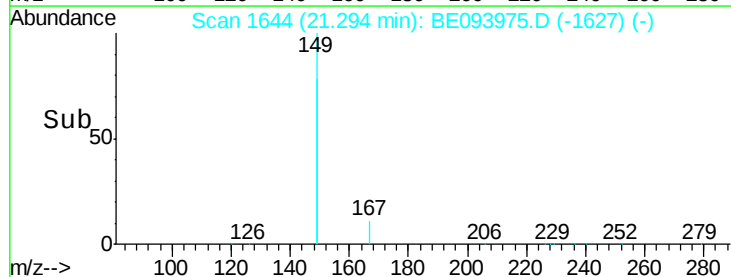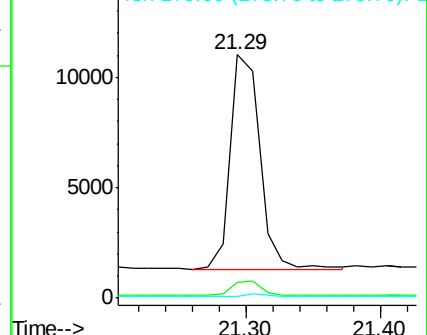

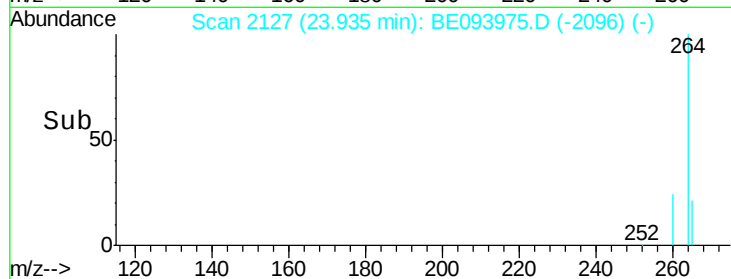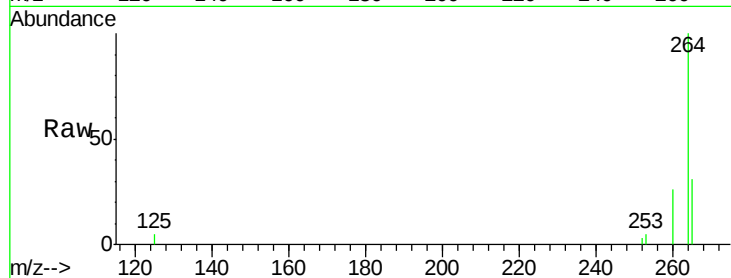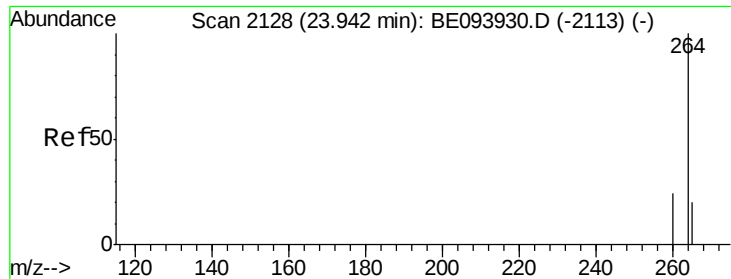

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.93 min Scan# 2127

Delta R.T. -0.01 min

Lab File: BE093975.D

Acq: 11 Sep 2017 22:42

Instrument :

BNA_E

ClientSampleId :

KY038PS033-170906

Tgt Ion: 264 Resp: 14210

Ion Ratio Lower Upper

264 100

260 25.7 20.0 30.0

265 31.0 24.0 36.0

