


Data Path : Z:\HPCHEM1\BNA_E\Data\BE091117\
 Data File : BE093953.D
 Acq On : 11 Sep 2017 9:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 13:34:56 2017

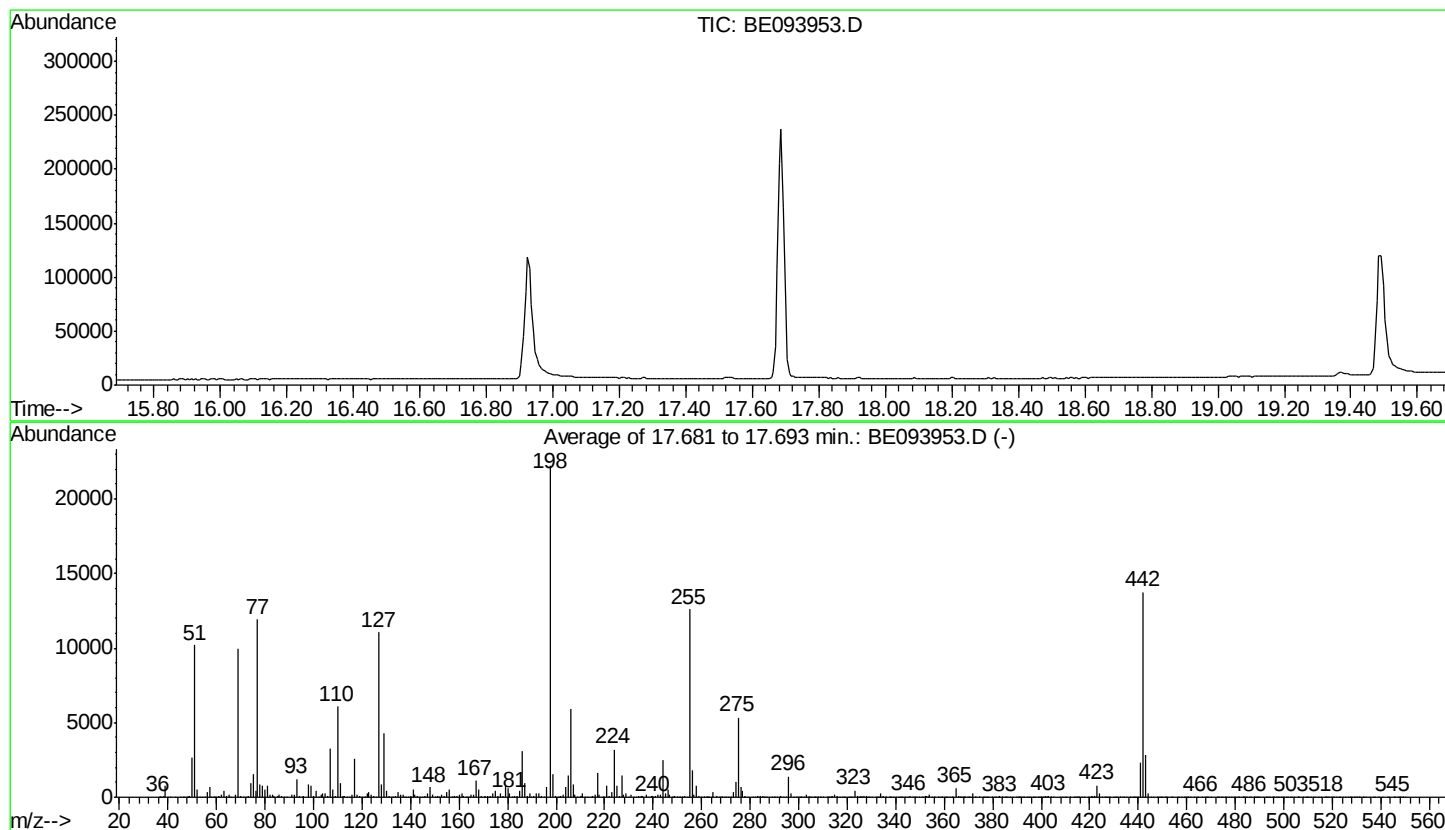

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	10201	PASS
68	69	0.00	2	1.4	143	PASS
69	198	0.00	100	44.9	9973	PASS
70	69	0.00	2	0.6	63	PASS
127	198	10	80	49.7	11049	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22231	PASS
199	198	5	9	7.0	1560	PASS
275	198	10	60	24.1	5364	PASS
365	198	1	100	2.7	609	PASS
441	442	0.01	24	17.1	2354	PASS
442	198	50	100	61.9	13754	PASS
443	442	15	24	20.6	2836	PASS