


Data Path : Z:\HPCHEM1\BNA_E\Data\BE091117\
 Data File : BE093972.D
 Acq On : 11 Sep 2017 20:52
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 13:34:56 2017

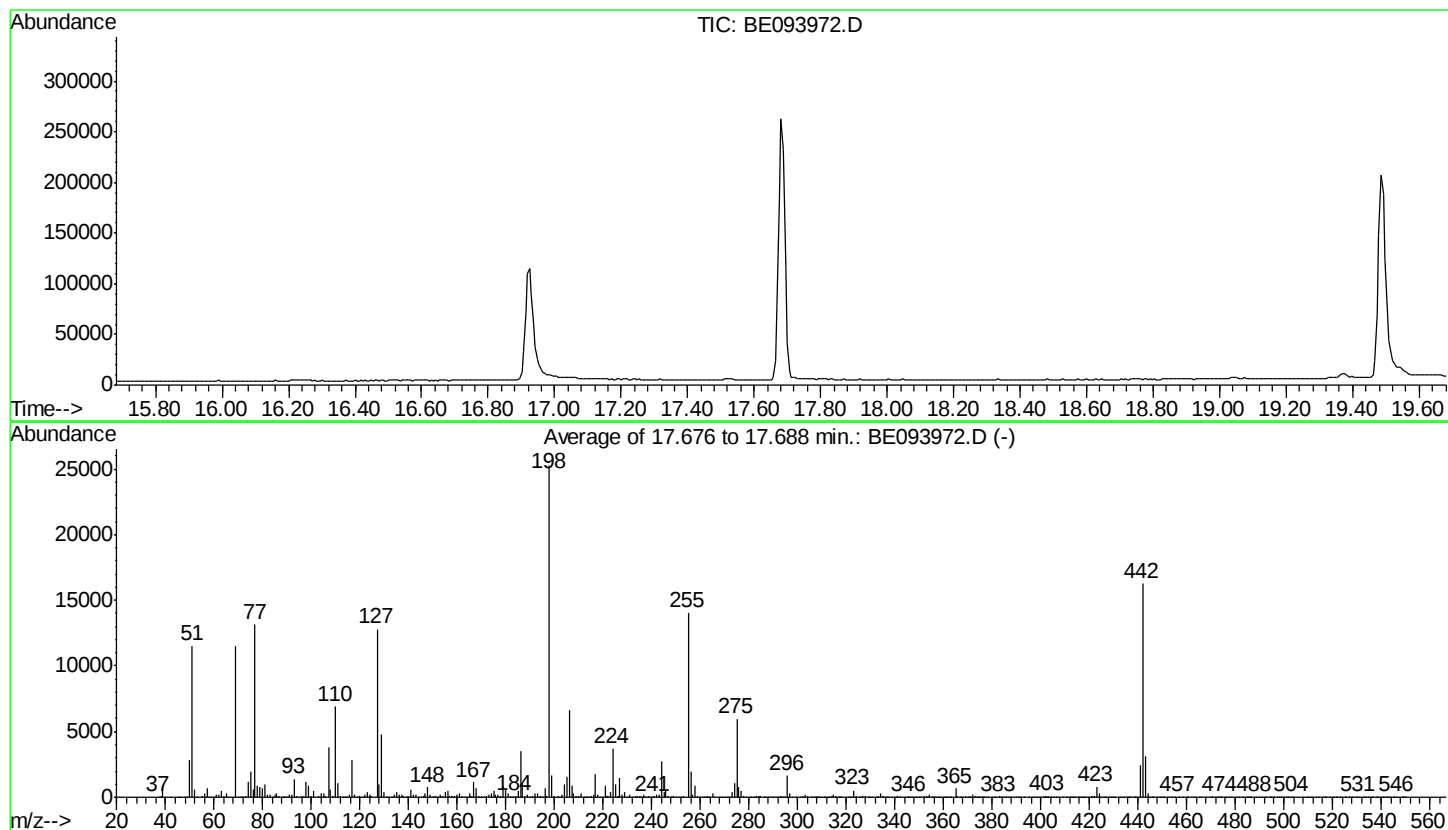

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.8	11553	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.6	11515	PASS
70	69	0.00	2	0.4	51	PASS
127	198	10	80	50.6	12772	PASS
197	198	0.00	2	0.4	98	PASS
198	198	100	100	100.0	25250	PASS
199	198	5	9	6.7	1682	PASS
275	198	10	60	23.7	5980	PASS
365	198	1	100	2.6	658	PASS
441	442	0.01	24	14.8	2404	PASS
442	198	50	100	64.3	16240	PASS
443	442	15	24	19.3	3138	PASS