
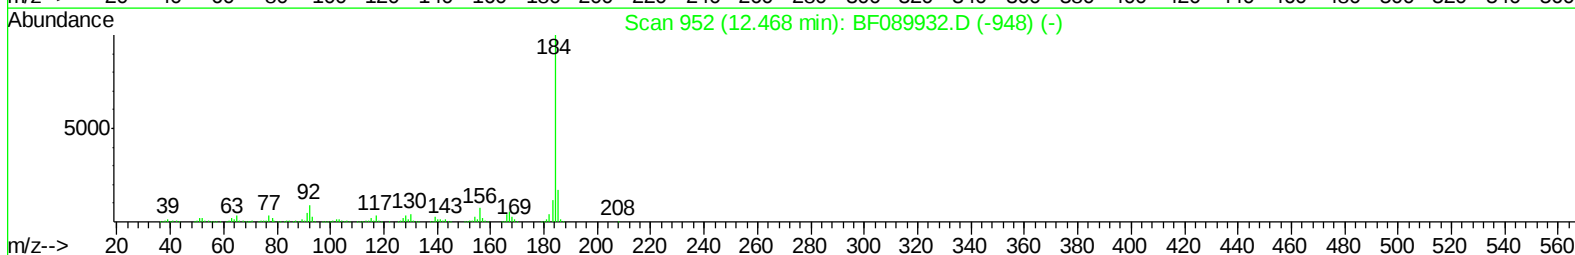
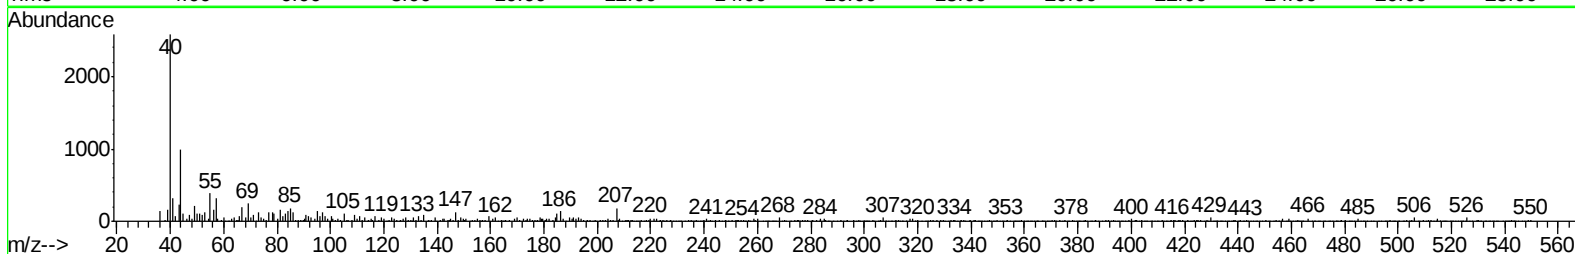


Data Path : Z:\HPCHEM1\BNA E\Data\BE091216\
 Data File : BE092368.D
 Acq On : 12 Sep 2016 8:47
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 17:01:07 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF083116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 08 16:07:52 2016
 Response via : Initial Calibration

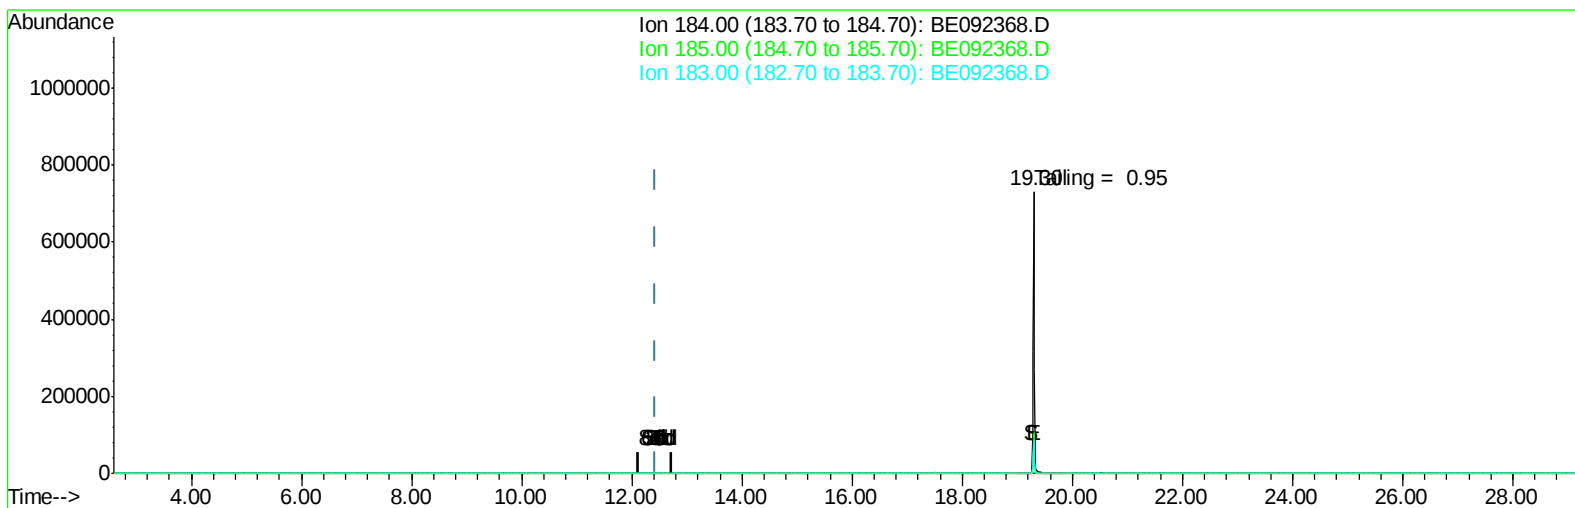

TIC: BE092368.D

(76) Benzidine




12.488min (+0.043) 29.70ng

response 54

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	212.96#
183.00	12.00	40.74#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE091216\
Data File : BE092368.D
Acq On : 12 Sep 2016 8:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 17:01:07 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 08 16:07:52 2016
Response via : Initial Calibration

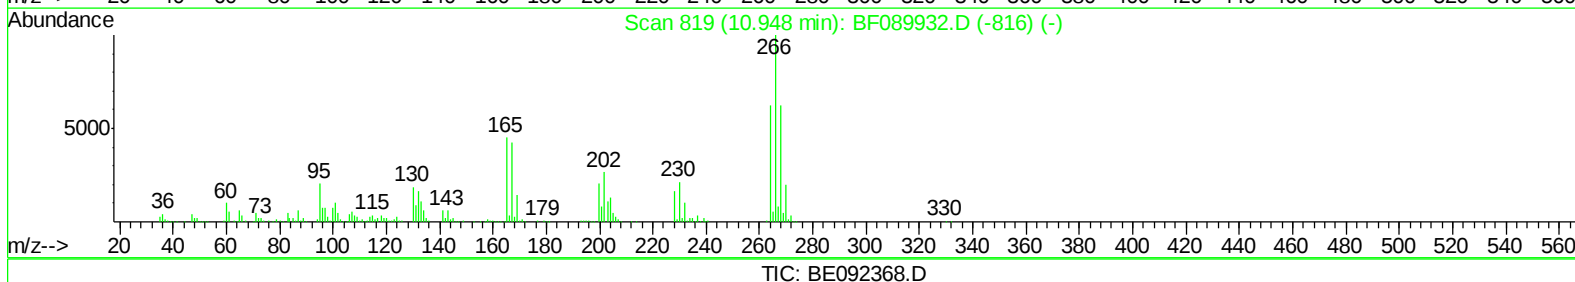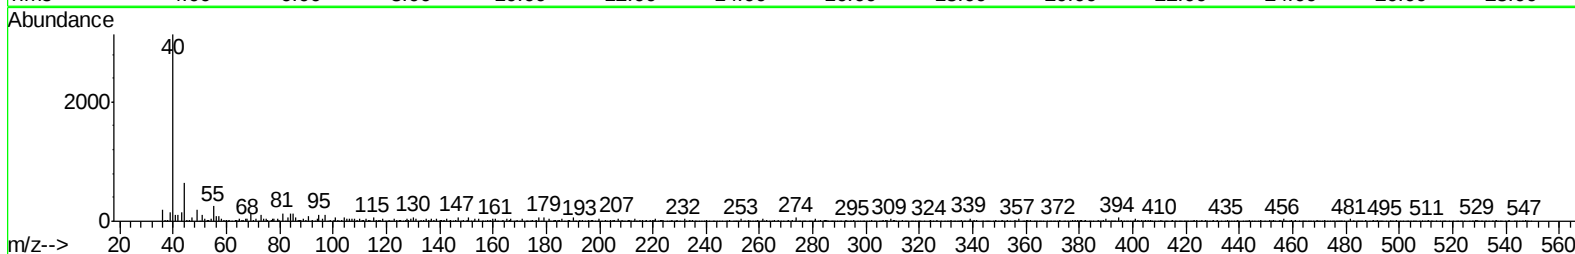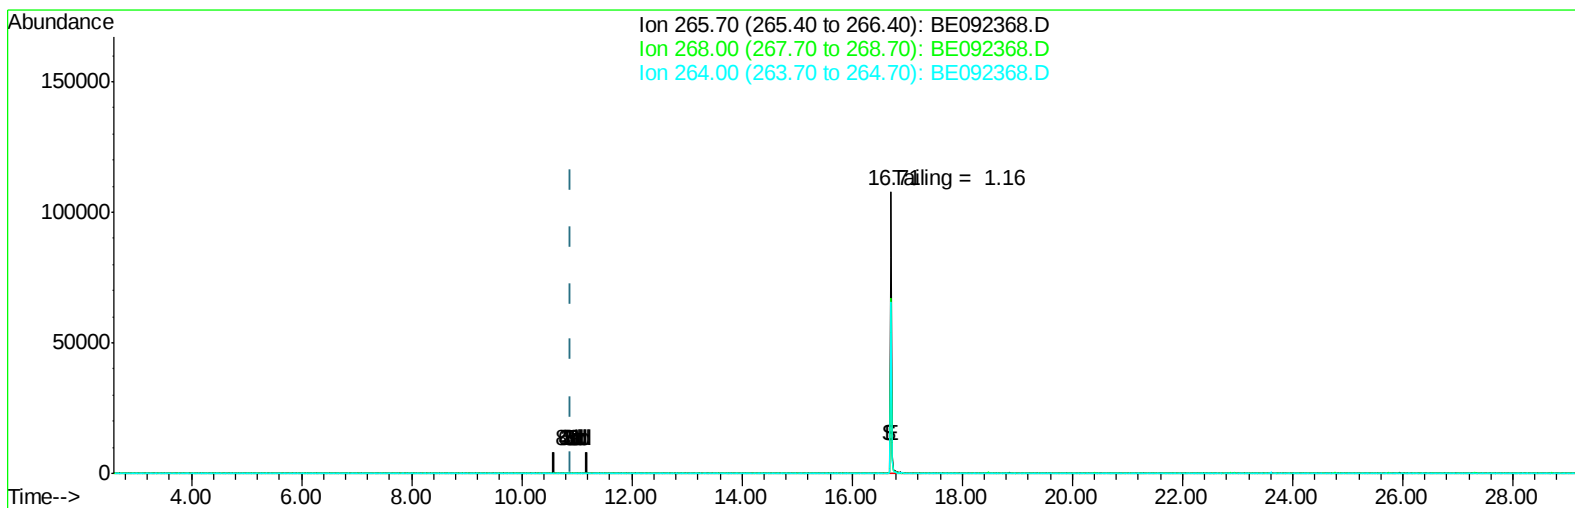

(69) Pentachlorophenol (C)
10.943min (+0.029) 186.51ng
response 15

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	9.09#
264.00	63.20	40.91#
0.00	0.00	0.00