


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091216\
 Data File : BE092368.D
 Acq On : 12 Sep 2016 8:47
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 02 19:34:51 2016

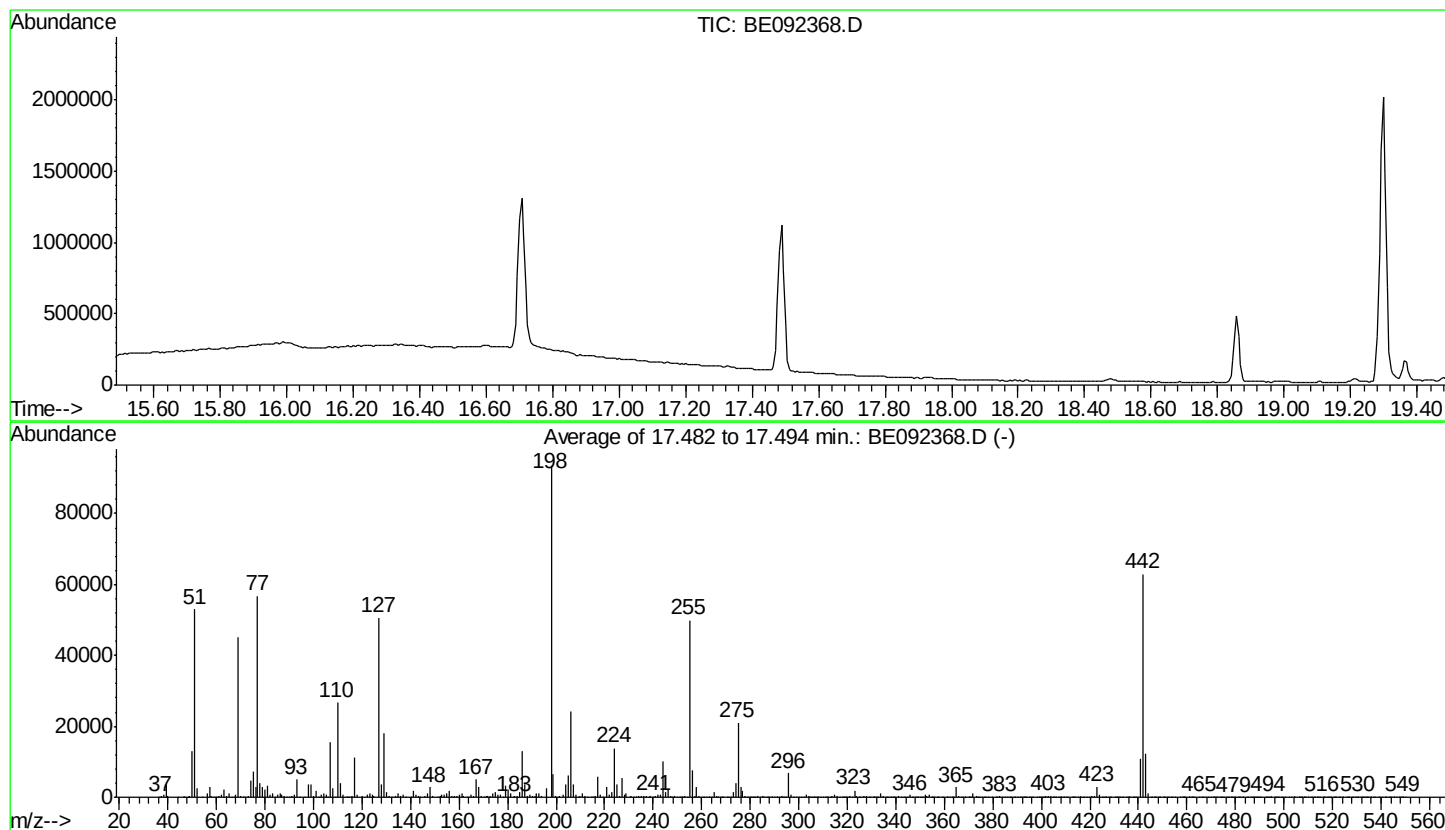

AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.7	53015	PASS
68	69	0.00	2	1.4	645	PASS
69	198	0.00	100	48.1	44979	PASS
70	69	0.00	2	0.6	280	PASS
127	198	10	80	54.2	50737	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93549	PASS
199	198	5	9	7.0	6528	PASS
275	198	10	60	22.4	20970	PASS
365	198	1	100	3.0	2804	PASS
441	442	0.01	24	17.0	10725	PASS
442	198	50	100	67.3	62925	PASS
443	442	15	24	19.4	12182	PASS