

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091218\
 Data File : BE097456.D
 Acq On : 12 Sep 2018 18:25
 Operator : SJ/JU
 Sample : PB112710BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Sep 13 01:52:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 13 01:51:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	961	0.40	ng/ul	0.00
2) Naphthalene-d8	10.12	136	5276	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	3688	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.86	188	668258	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.97
20) Perylene-d12	23.20	264	15653	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	2681	0.33	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.01	166	957	0.072	ng/ul#	22
23) Benzo(a)pyrene	23.06	252	2602	0.067	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091218\
Data File : BE097456.D
Acq On : 12 Sep 2018 18:25
Operator : SJ/JU
Sample : PB112710BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Sep 13 01:52:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 13 01:51:24 2018
Response via : Initial Calibration




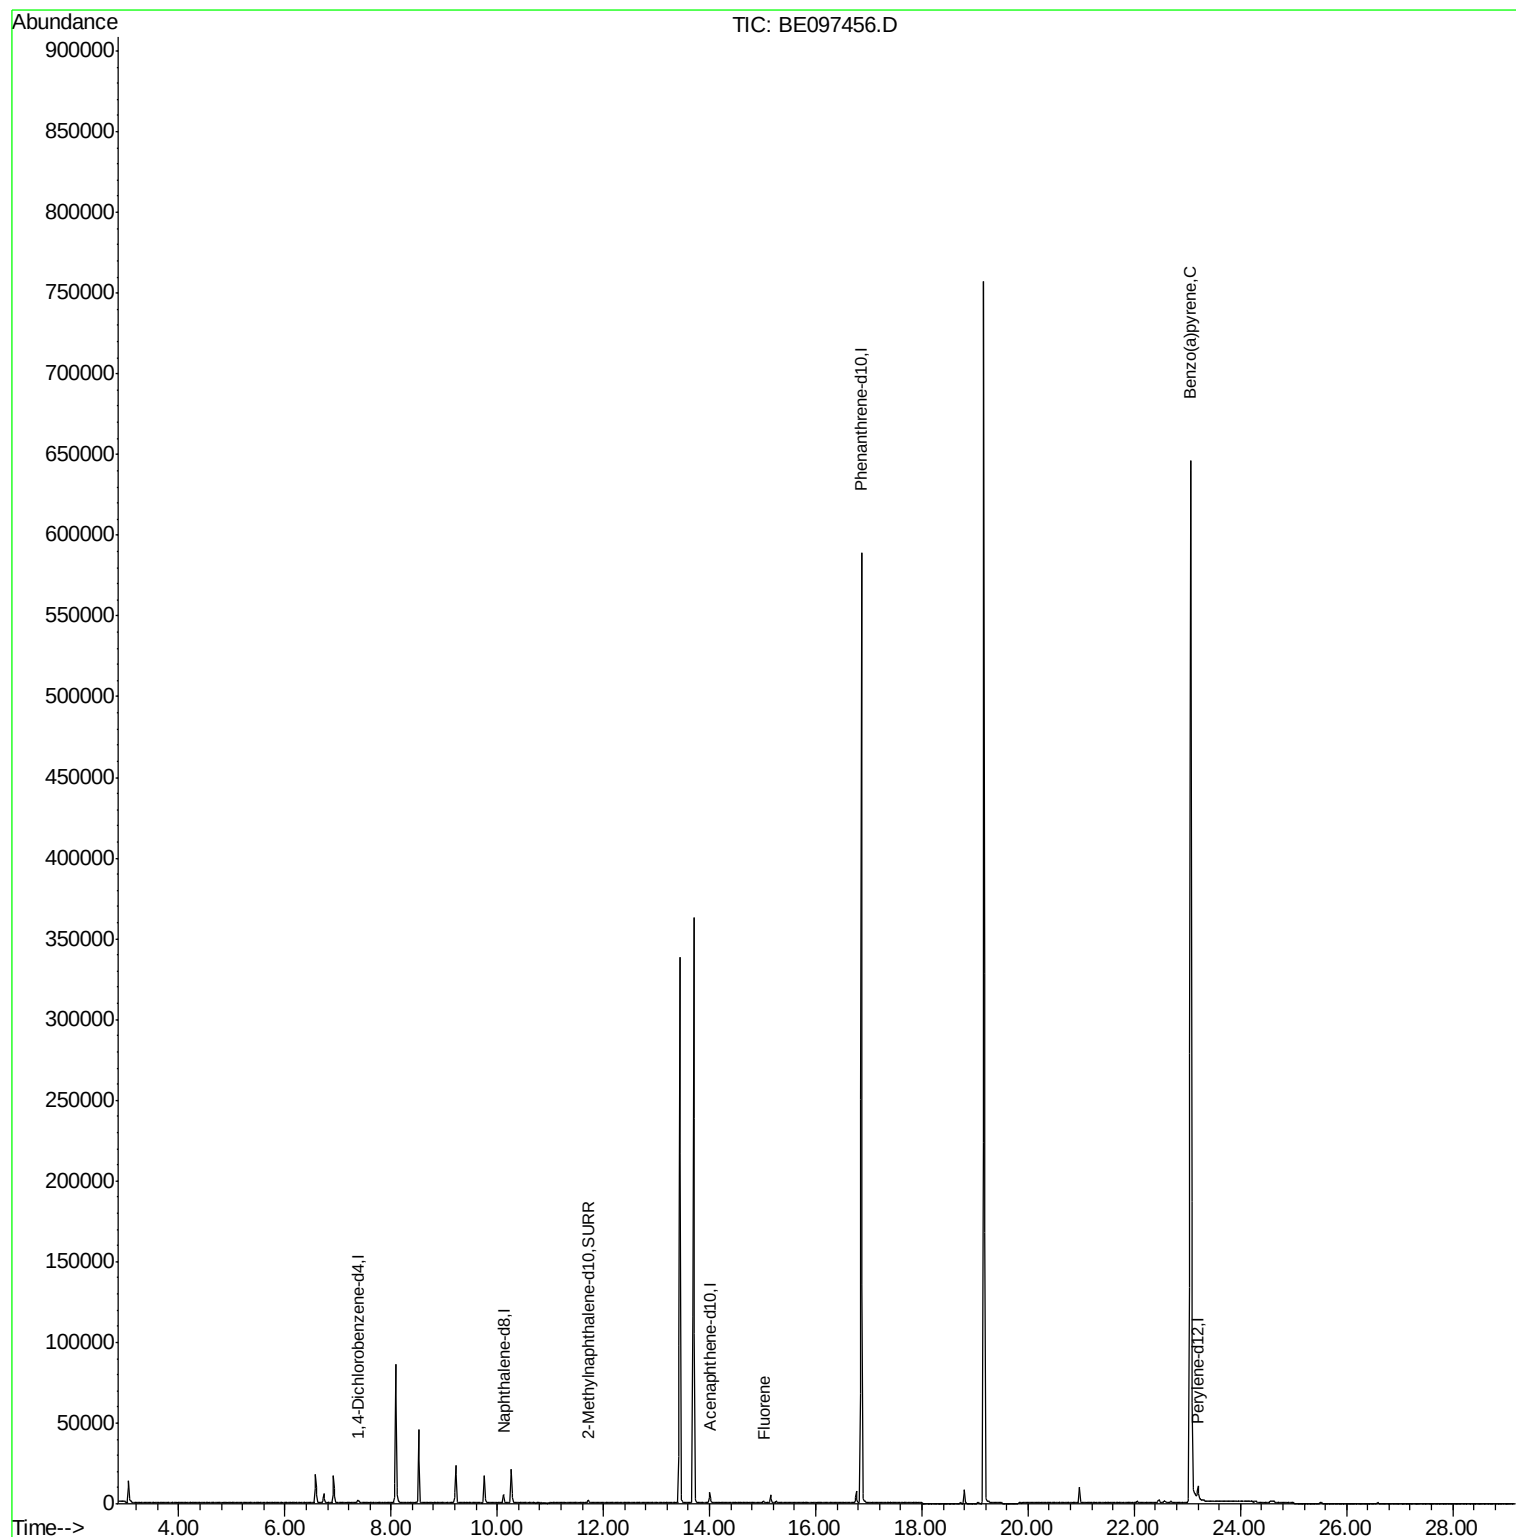


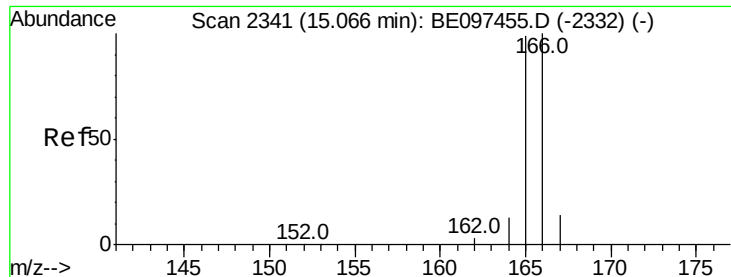

#9
Fluorene
 Concen: 0.072 ng/ul
 RT: 15.01 min Scan# 2330
 Delta R.T. -0.05 min
 Lab File: BE097456.D
 Acq: 12 Sep 2018 18:25

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:166 Resp: 957
 Ion Ratio Lower Upper
 166 100
 165 10.4 73.4 110.2#
 167 36.5 14.6 22.0#

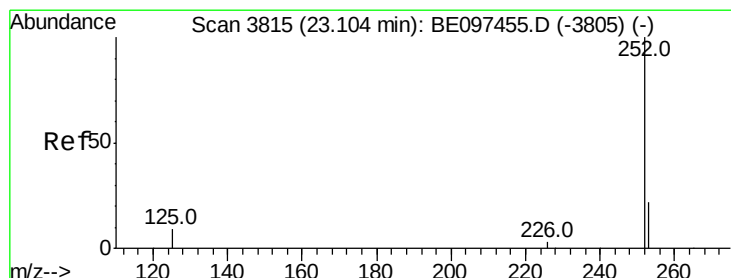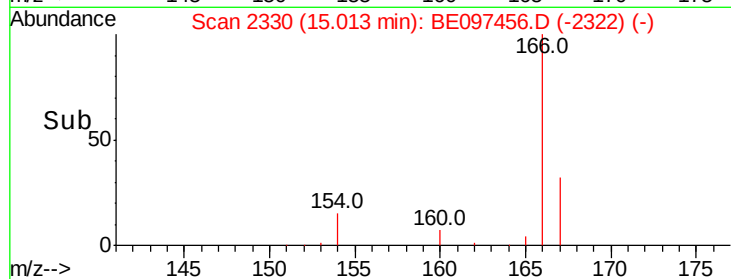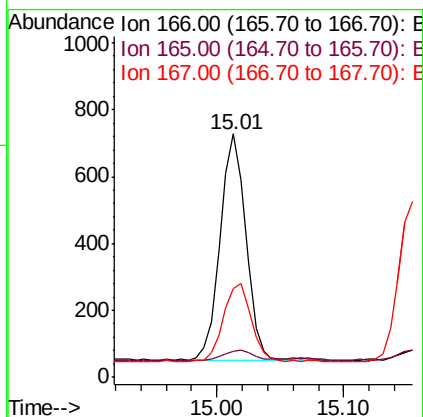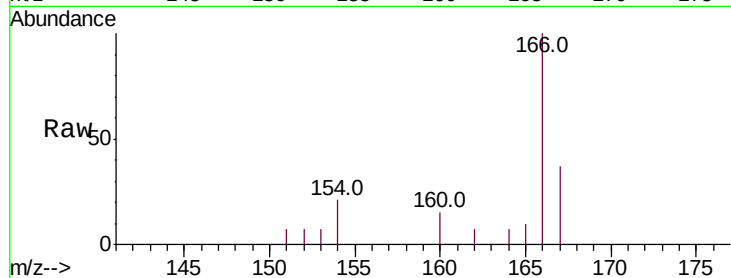

#23
Benzo(a)pyrene
 Concen: 0.067 ng/ul
 RT: 23.06 min Scan# 3806
 Delta R.T. -0.04 min
 Lab File: BE097456.D
 Acq: 12 Sep 2018 18:25

Tgt Ion:252 Resp: 2602
 Ion Ratio Lower Upper
 252 100
 253 31.8 28.5 42.7
 125 20.6 18.1 27.1

