

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091218\
 Data File : BE097457.D
 Acq On : 12 Sep 2018 19:00
 Operator : SJ/JU
 Sample : J4792-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Sep 13 01:53:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 13 01:51:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	1028	0.40	ng/ul	0.00
2) Naphthalene-d8	10.12	136	5496	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	3668	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.86	188	392955	0.40	ng/ul	0.10
16) Chrysene-d12	21.08	240	17	0.40	ng/ul	0.11
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.20
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	1636	0.19	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.20	202	704	15.389	ng/ul#	94
18) Benzo(a)anthracene	21.00	228	316	7.236	ng/ul#	65
19) Chrysene	21.12	228	41	0.815	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091218\
Data File : BE097457.D
Acq On : 12 Sep 2018 19:00
Operator : SJ/JU
Sample : J4792-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Sep 13 01:53:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 13 01:51:24 2018
Response via : Initial Calibration




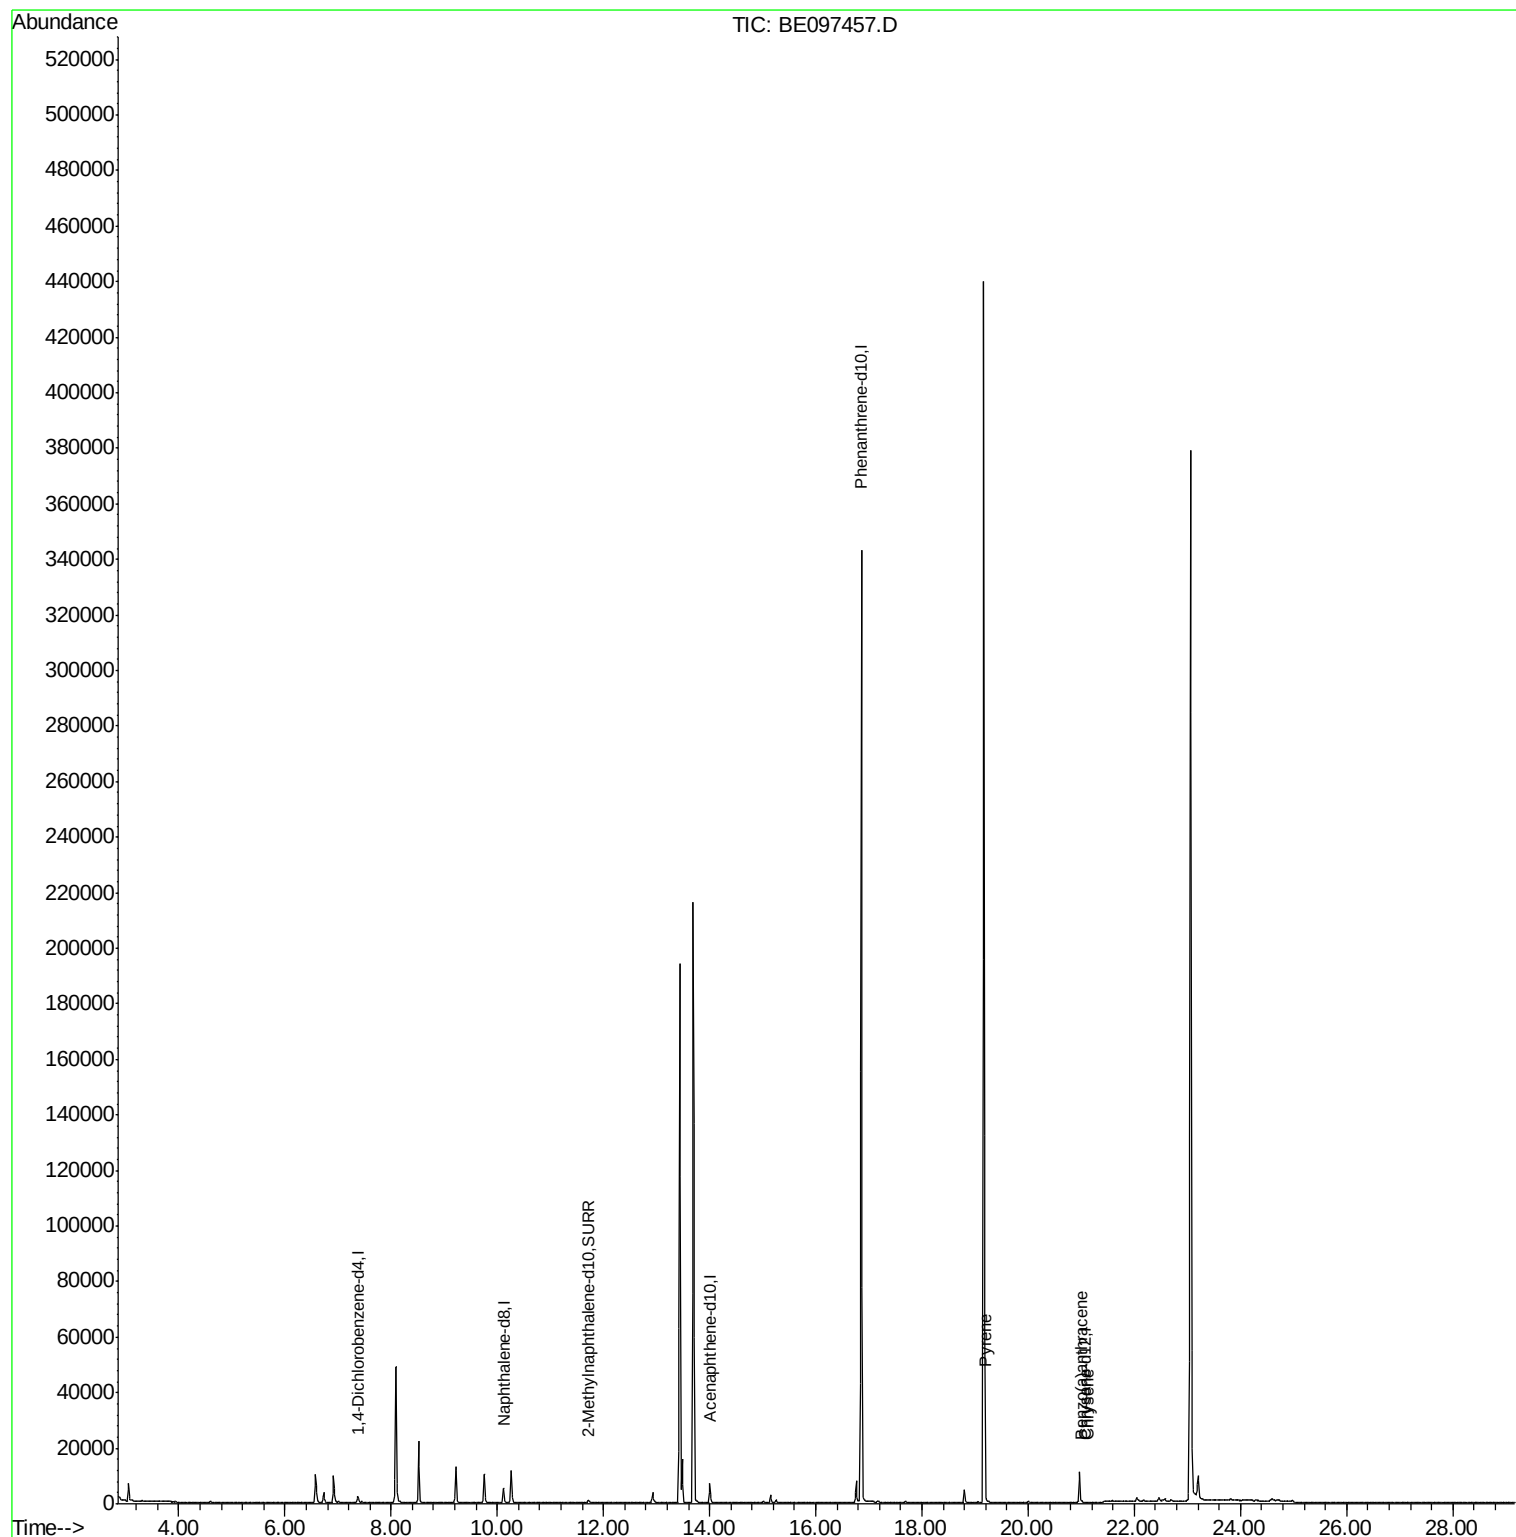


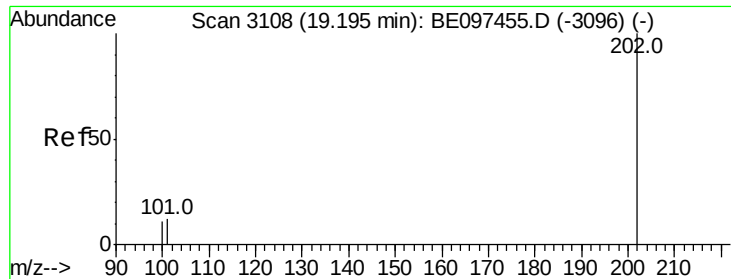

#17
 Pvrene
 Concen: 15.389 ng/ul
 RT: 19.20 min Scan# 3106
 Delta R.T. 0.00 min
 Lab File: BE097457.D
 Acq: 12 Sep 2018 19:00




Instrument :
 BNA_E
 ClientSampleId :




Tot Ion:202 Resp: 704
 Ion Ratio Lower Upper
 202 100
 101 22.4 18.2 27.4
 100 25.3 15.6 23.4#

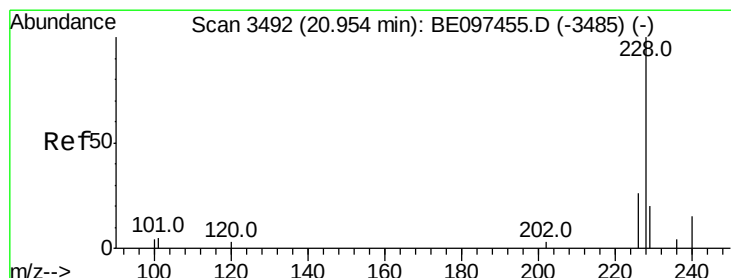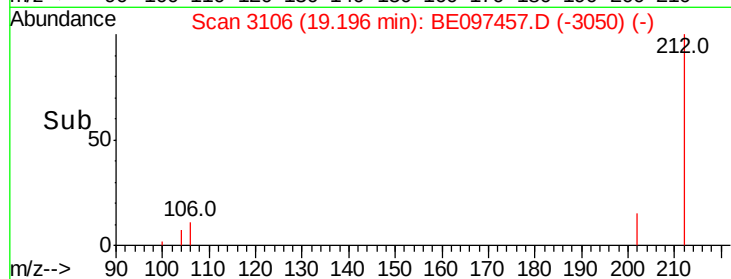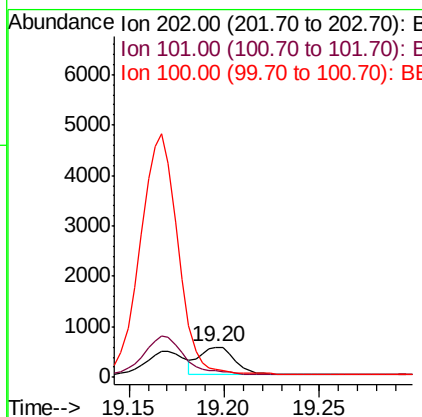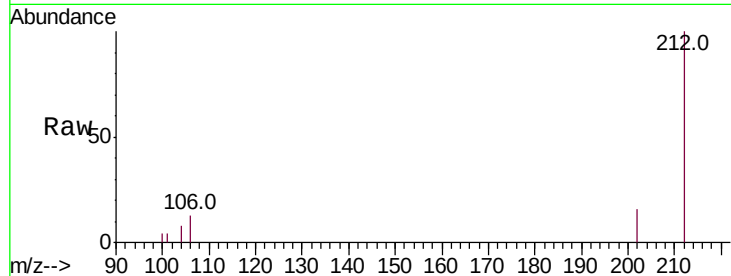

#18
 Benzo(a)anthracene
 Concen: 7.236 ng/ul
 RT: 21.00 min Scan# 3499
 Delta R.T. 0.05 min
 Lab File: BE097457.D
 Acq: 12 Sep 2018 19:00

Tgt Ion:228 Resp: 316
 Ion Ratio Lower Upper
 228 100
 229 39.9 22.8 34.2#
 226 46.4 17.0 25.6#

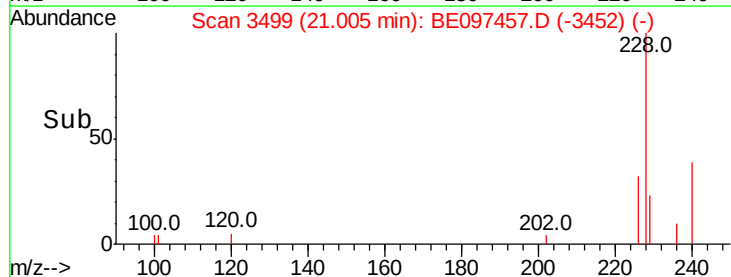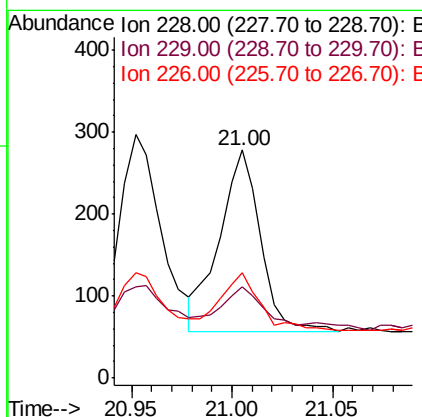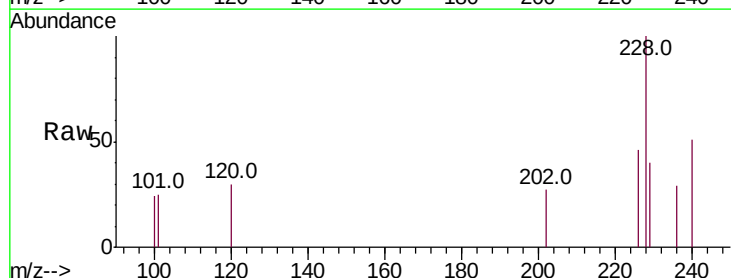

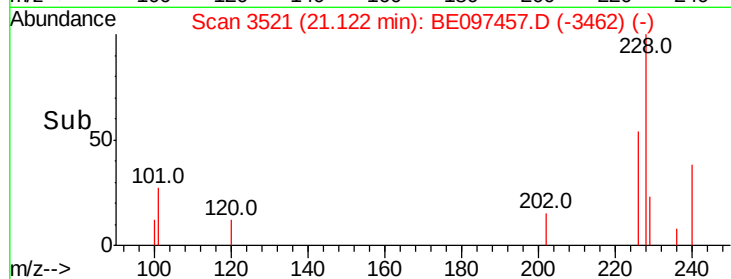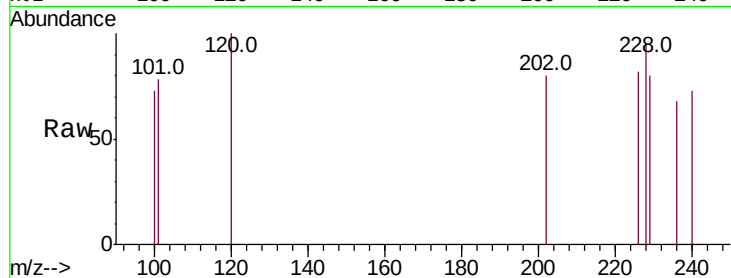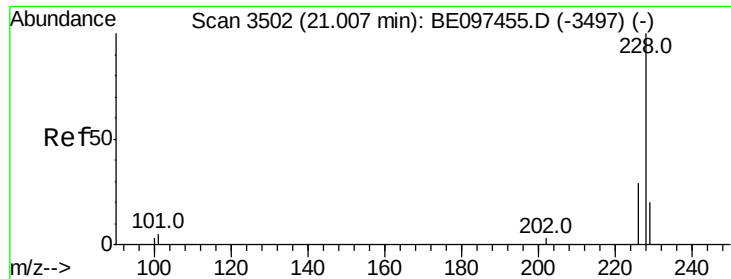

#19

Chrysene

Concen: 0.815 ng/ul

RT: 21.12 min Scan# 3521

Delta R.T. 0.11 min

Lab File: BE097457.D

Acq: 12 Sep 2018 19:00

Instrument :

BNA_E

ClientSampleId :

Tot Ion:228 Resp: 41

Ion Ratio Lower Upper

228 100

226 86.4 23.4 35.0#

229 84.0 17.7 26.5#

