

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091218\
 Data File : BE097458.D
 Acq On : 12 Sep 2018 19:39
 Operator : SJ/JU
 Sample : J4792-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Sep 13 01:53:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 13 01:51:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	965	0.40	ng/ul	0.00
2) Naphthalene-d8	10.12	136	5398	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	3943	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.86	188	572196	0.40	ng/ul	0.10
16) Chrysene-d12	21.10	240	35	0.40	ng/ul	0.13
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.20
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.71	152	2485	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.20	202	1269	13.474	ng/ul	97
18) Benzo(a)anthracene	21.10	228	101	1.123	ng/ul#	1
19) Chrysene	21.12	228	71	0.685	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091218\
Data File : BE097458.D
Acq On : 12 Sep 2018 19:39
Operator : SJ/JU
Sample : J4792-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Sep 13 01:53:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE082918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 13 01:51:24 2018
Response via : Initial Calibration




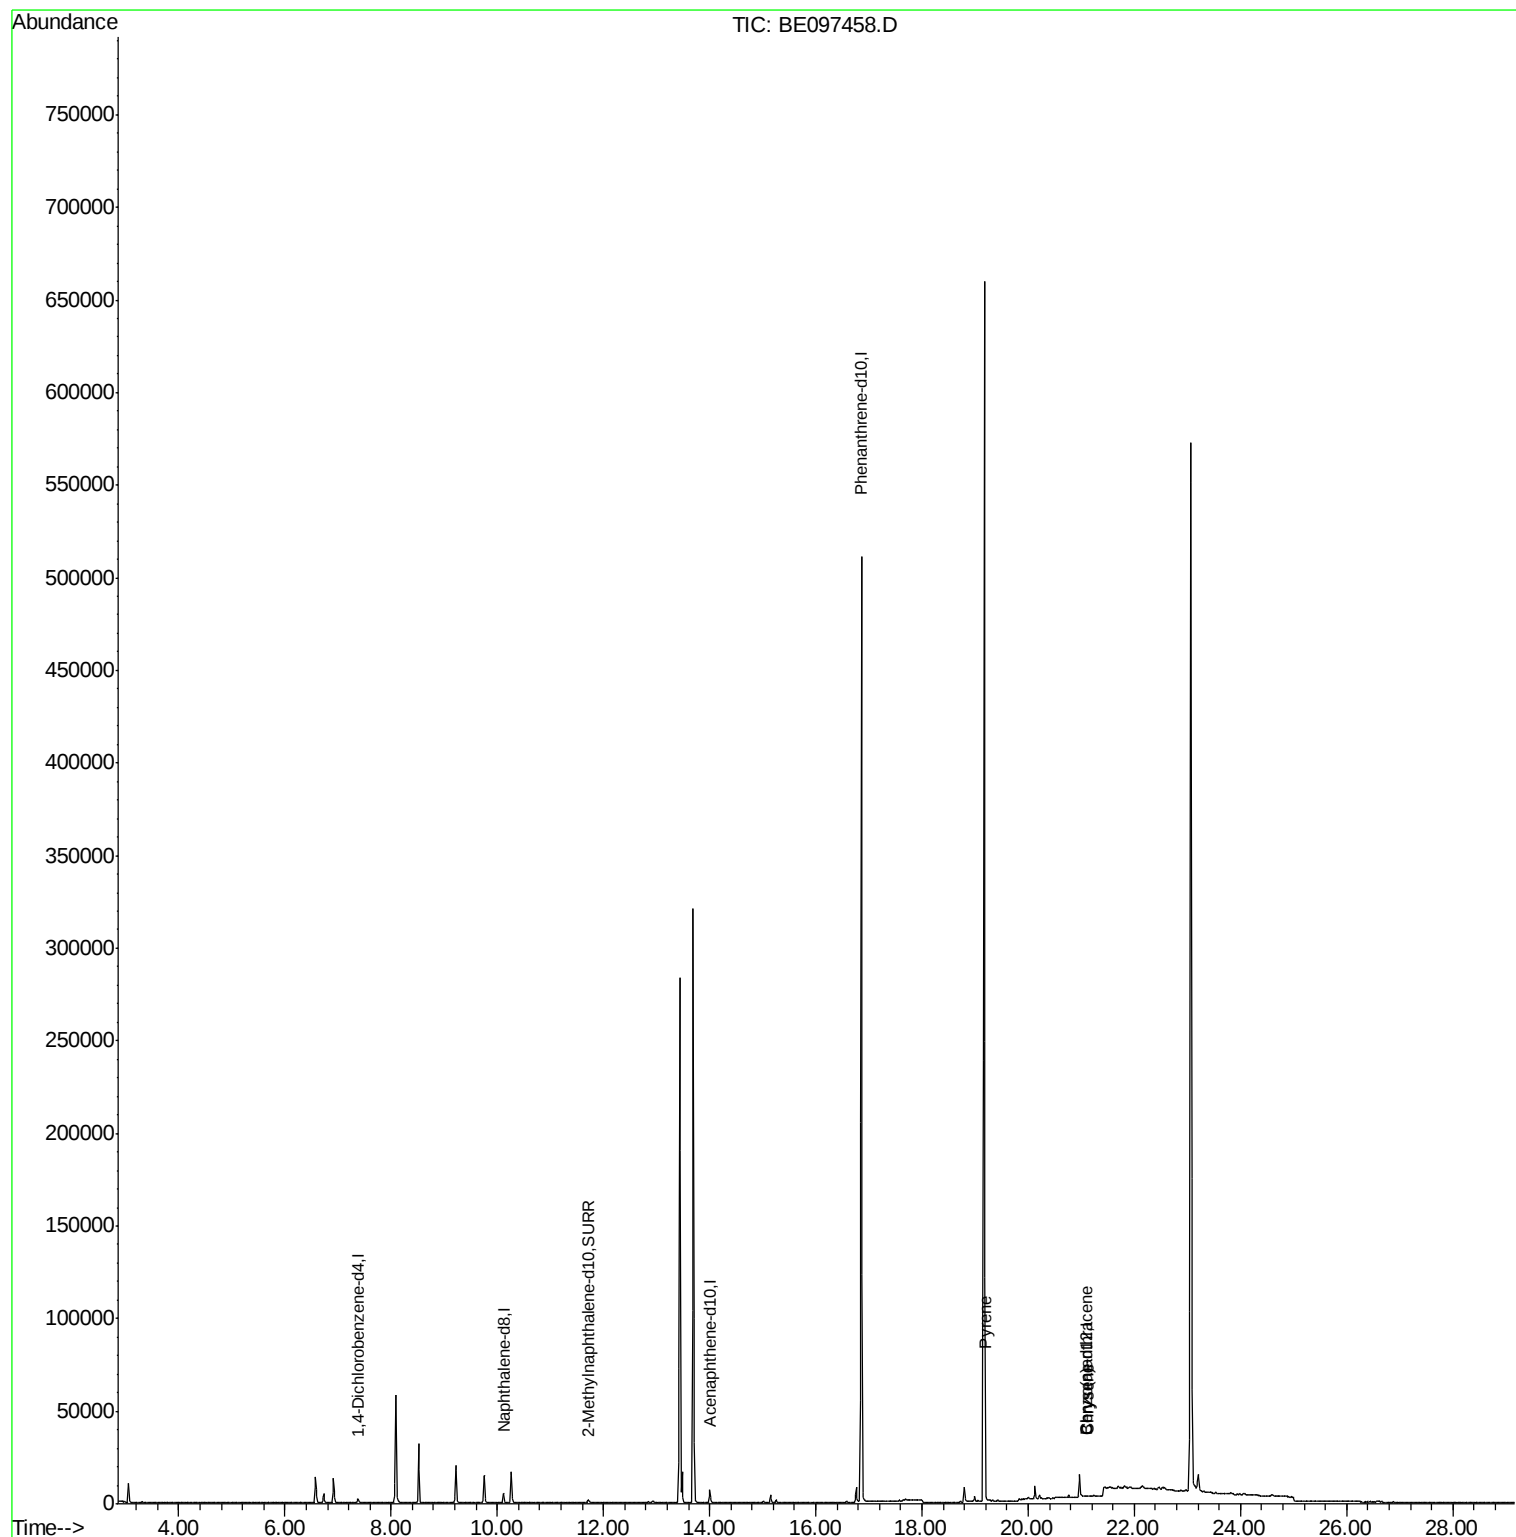


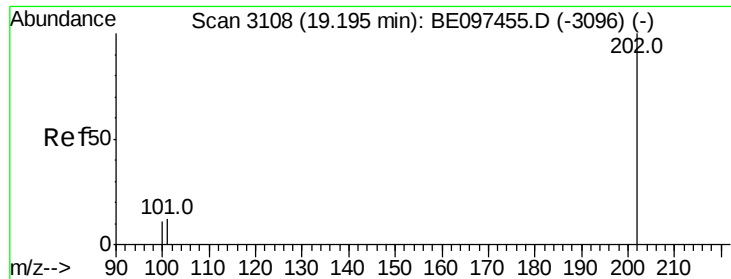

#17
Pvrene
Concen: 13.474 ng/ul
RT: 19.20 min Scan# 3106
Delta R.T. 0.00 min
Lab File: BE097458.D
Acq: 12 Sep 2018 19:39




Instrument :
BNA_E
ClientSampleId :




Tot Ion:202 Resp: 1269
Ion Ratio Lower Upper
202 100
101 21.1 18.2 27.4
100 20.5 15.6 23.4

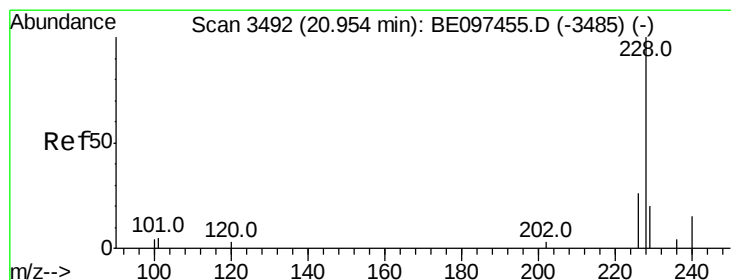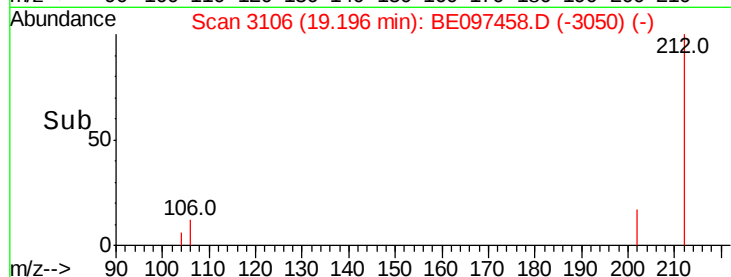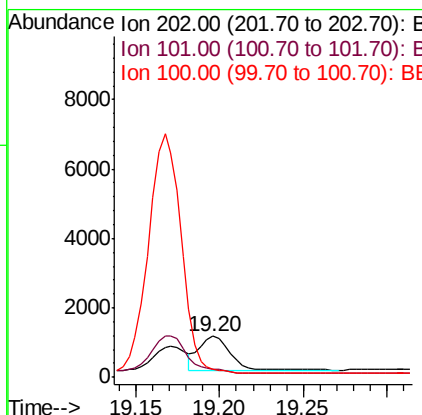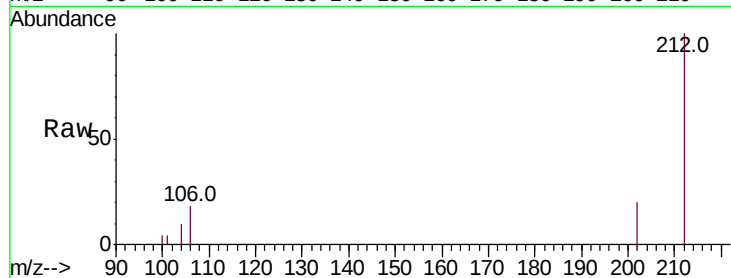

#18
Benzo(a)anthracene
Concen: 1.123 ng/ul
RT: 21.10 min Scan# 3516
Delta R.T. 0.14 min
Lab File: BE097458.D
Acq: 12 Sep 2018 19:39

Tgt Ion:228 Resp: 101
Ion Ratio Lower Upper
228 100
229 150.4 22.8 34.2#
226 98.2 17.0 25.6#

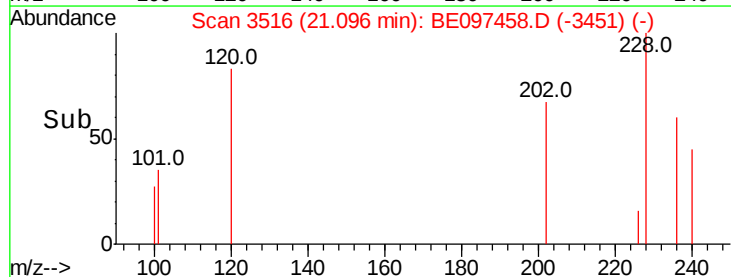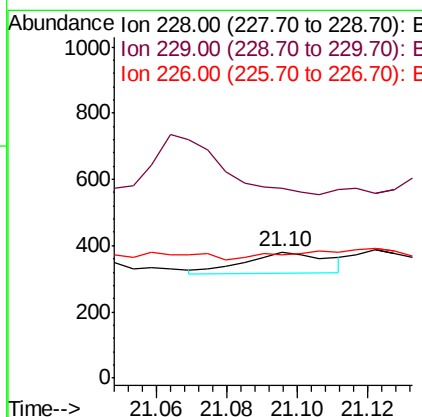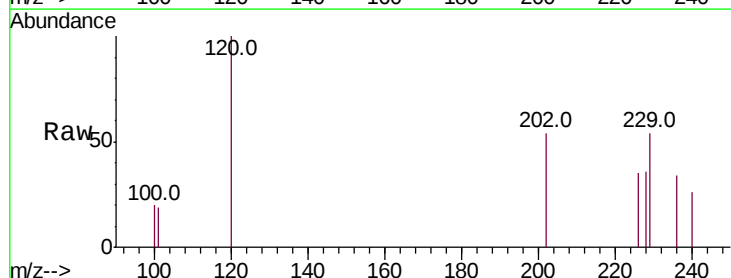

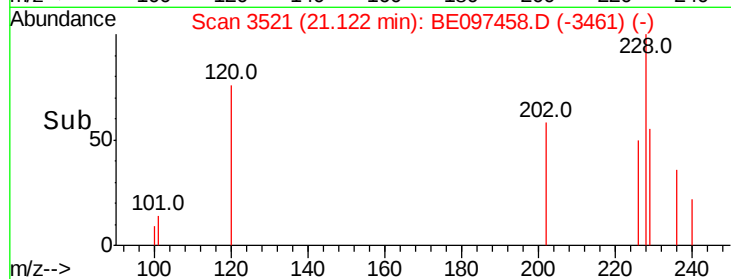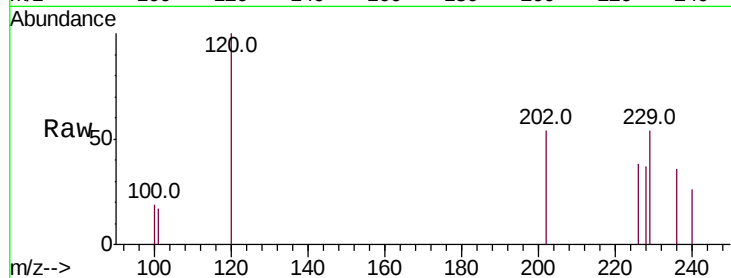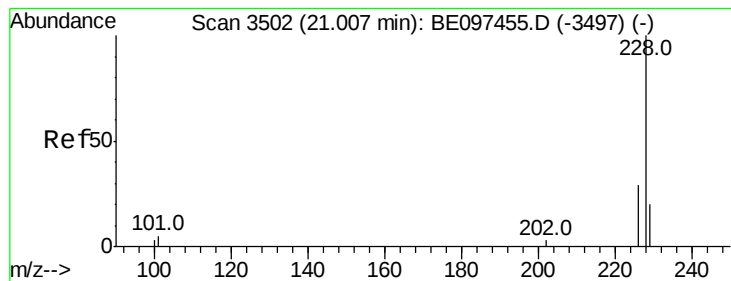

#19

Chrysene

Concen: 0.685 ng/ul

RT: 21.12 min Scan# 3521

Delta R.T. 0.12 min

Lab File: BE097458.D

Acq: 12 Sep 2018 19:39

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 228 Resp: 71

Ion Ratio Lower Upper

228 100

226 100.8 23.4 35.0#

229 143.9 17.7 26.5#

