
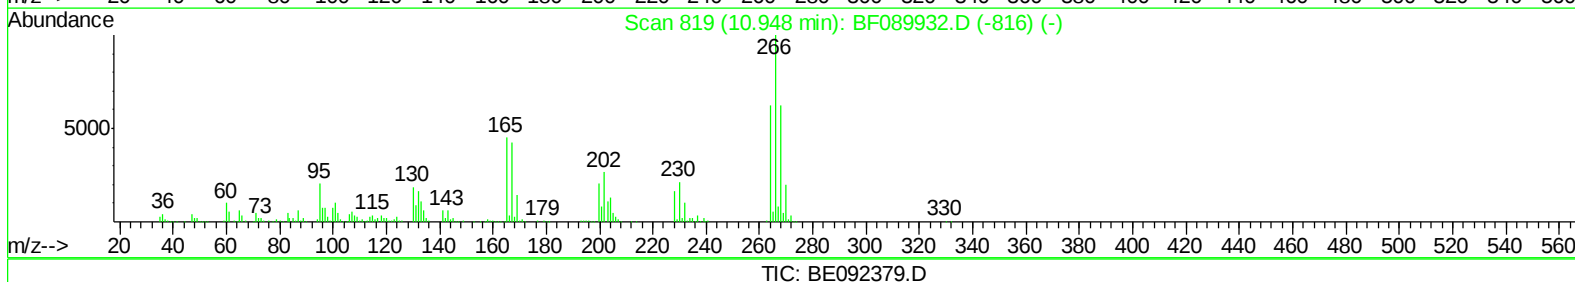
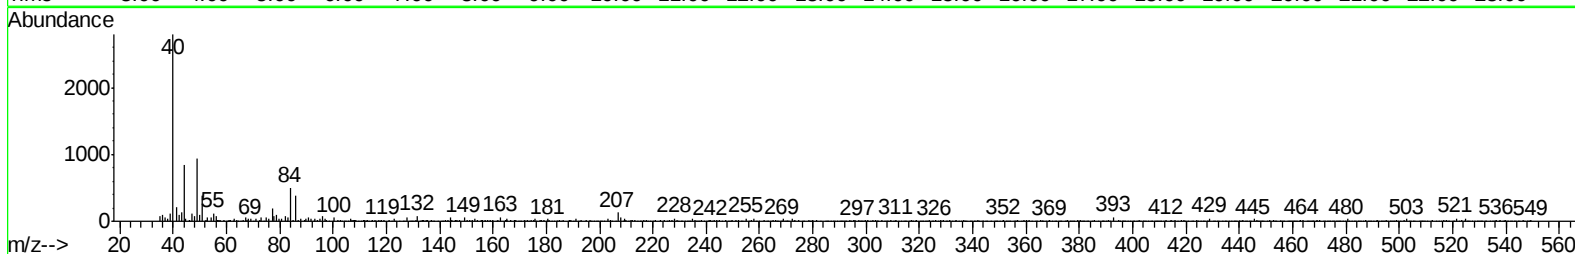


Data Path : Z:\HPCHEM1\BNA E\Data\BE091316\
Data File : BE092379.D
Acq On : 13 Sep 2016 11:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 17:50:56 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 08 16:07:52 2016
Response via : Initial Calibration

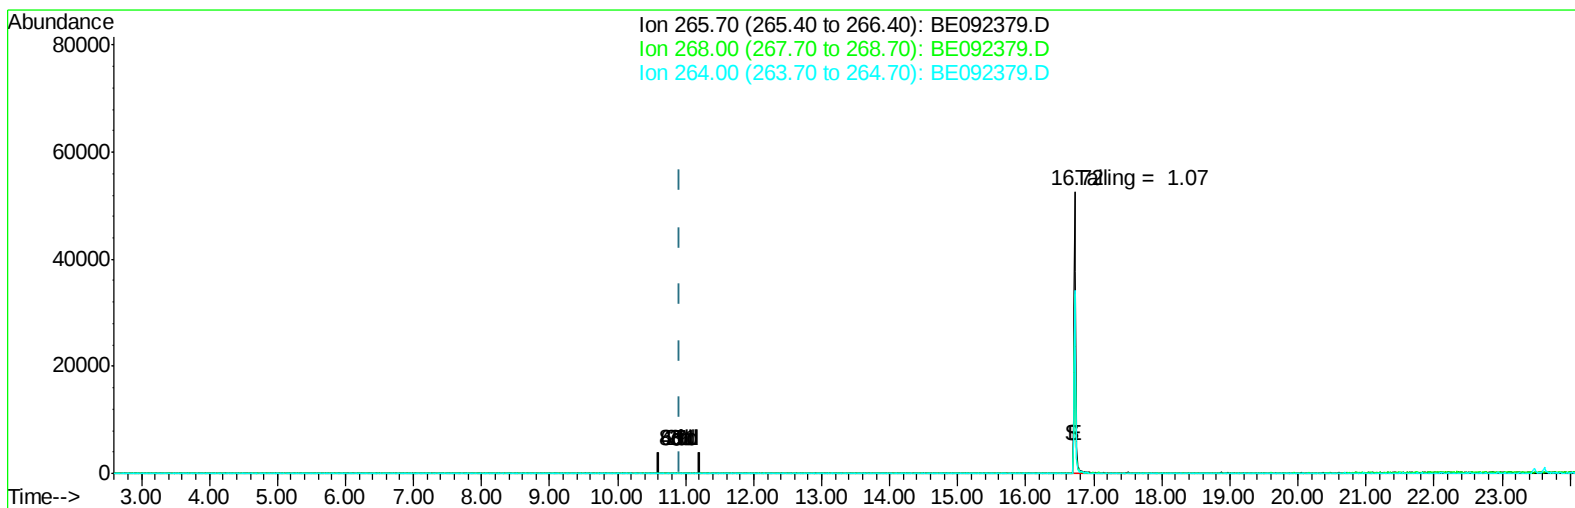

TIC: BE092379.D

(69) Pentachlorophenol (C)




11.086min (+0.172) 68.06ng

response 8

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	75.00
264.00	63.20	66.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE091316\
Data File : BE092379.D
Acq On : 13 Sep 2016 11:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 17:50:56 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 08 16:07:52 2016
Response via : Initial Calibration

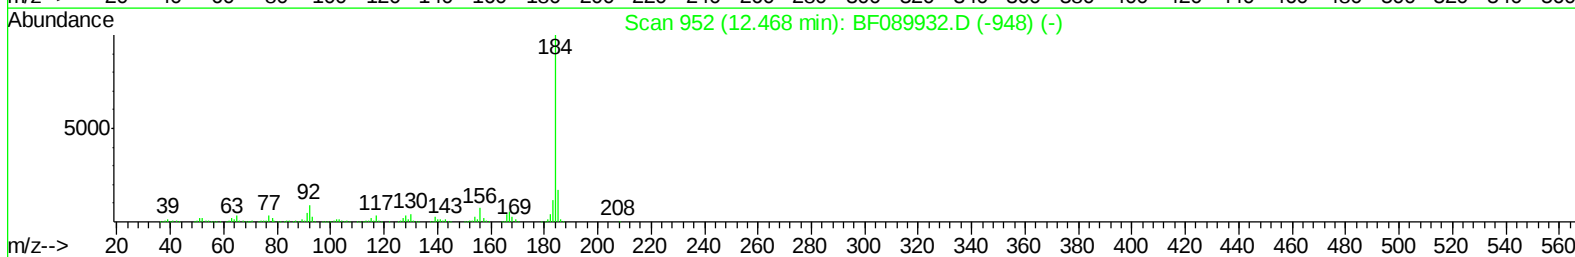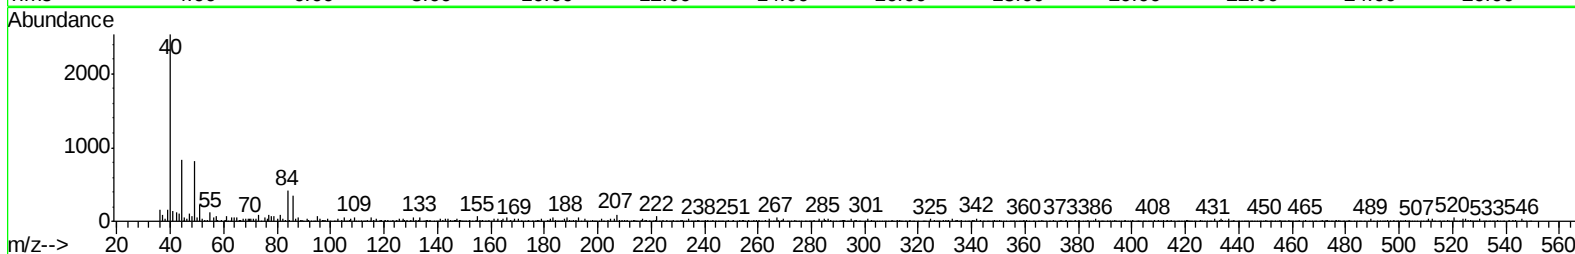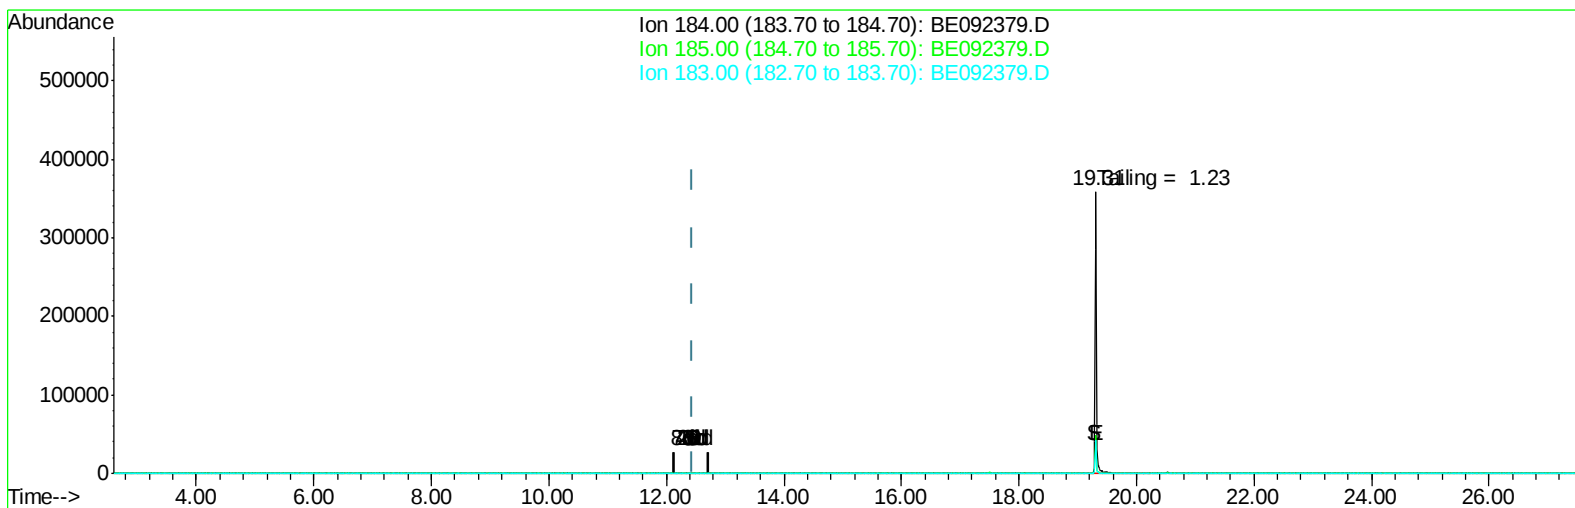

TIC: BE092379.D

(76) Benzidine

12.437min (-0.008) 41.48ng

response 11

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	17.39
183.00	12.00	195.65#
0.00	0.00	0.00