


Data Path : Z:\HPCHEM1\BNA E\DATA\BE091316\
 Data File : BE092379.D
 Acq On : 13 Sep 2016 11:20
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 02 19:34:51 2016

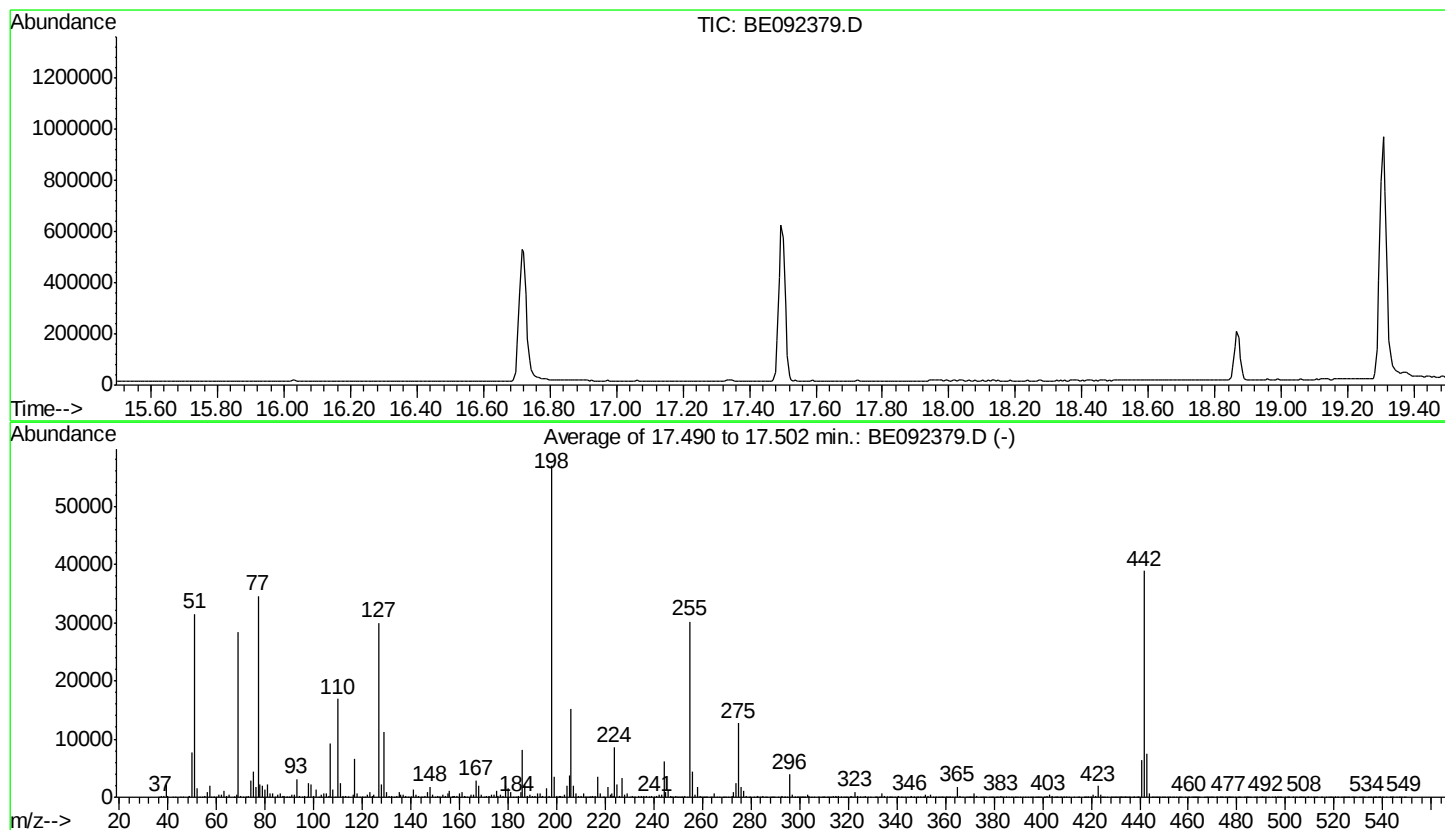

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2529

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.4	31540	PASS
68	69	0.00	2	1.8	501	PASS
69	198	0.00	100	49.8	28348	PASS
70	69	0.00	2	0.6	167	PASS
127	198	10	80	52.6	29955	PASS
197	198	0.00	2	0.4	219	PASS
198	198	100	100	100.0	56959	PASS
199	198	5	9	6.4	3633	PASS
275	198	10	60	22.4	12732	PASS
365	198	1	100	3.2	1798	PASS
441	442	0.01	24	16.6	6472	PASS
442	198	50	100	68.3	38879	PASS
443	442	15	24	19.2	7460	PASS