


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE091317\
 Data File : BE093980.D
 Acq On : 13 Sep 2017 9:13
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 13:34:56 2017

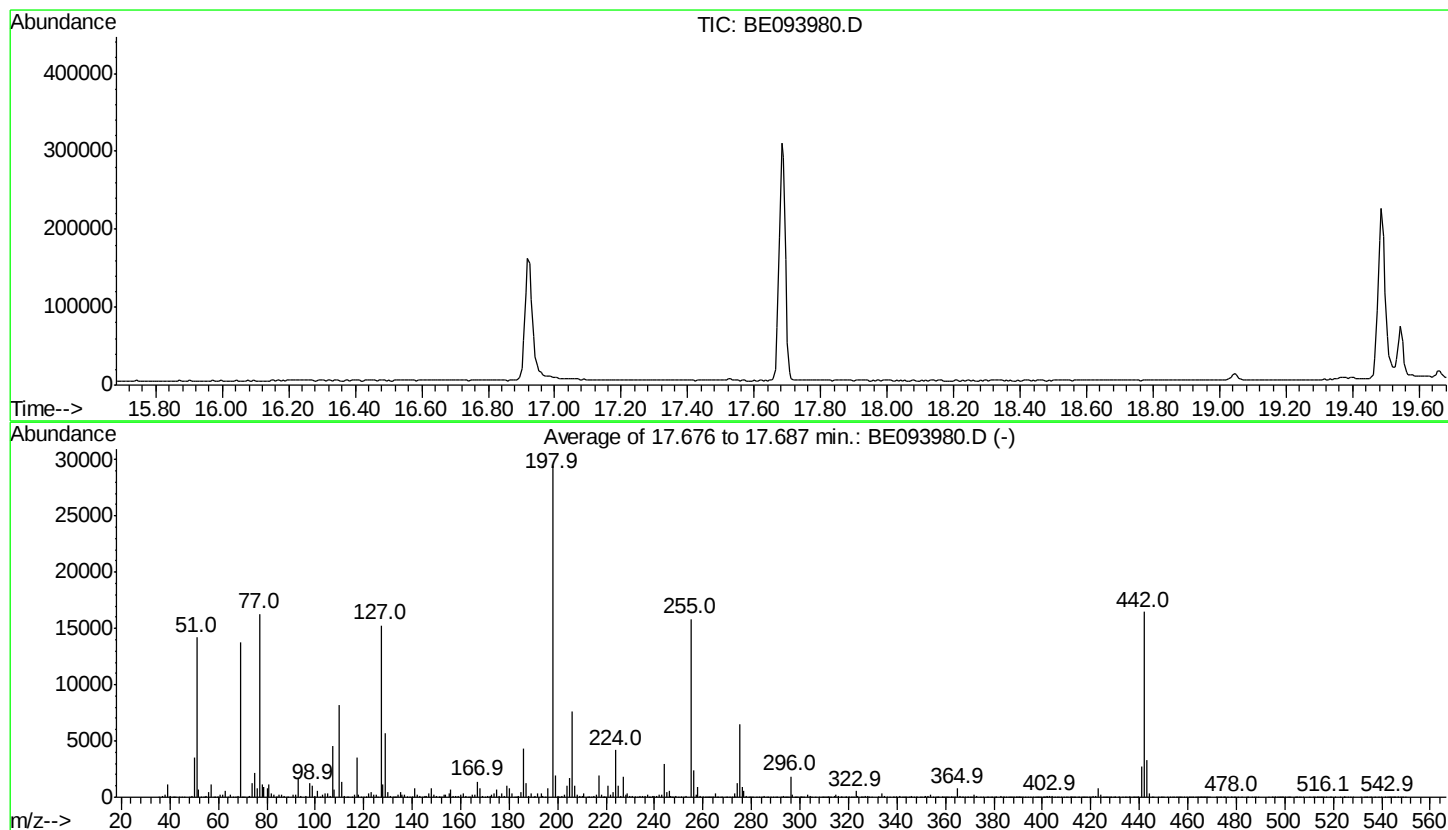

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.1	14170	PASS
68	69	0.00	2	0.8	105	PASS
69	198	0.00	100	46.8	13793	PASS
70	69	0.00	2	0.4	52	PASS
127	198	10	80	51.8	15258	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29466	PASS
199	198	5	9	6.6	1957	PASS
275	198	10	60	22.1	6524	PASS
365	198	1	100	2.5	747	PASS
441	442	0.01	24	16.7	2753	PASS
442	198	50	100	55.9	16484	PASS
443	442	15	24	20.0	3302	PASS