
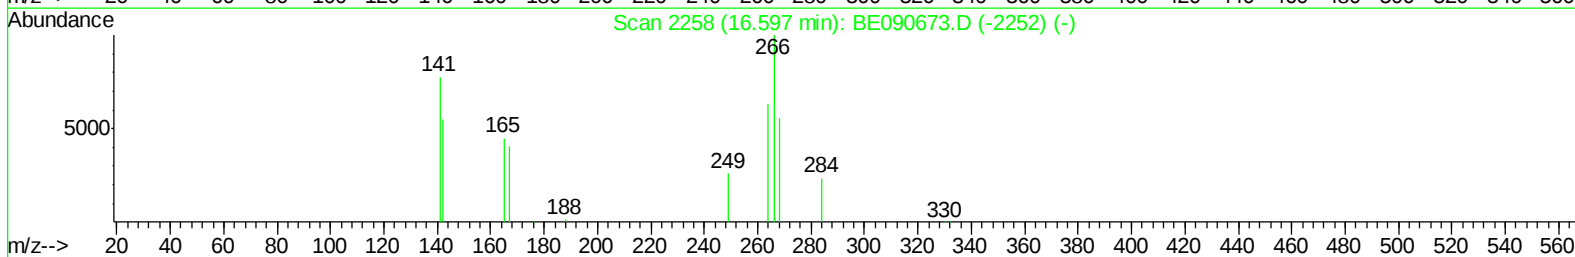
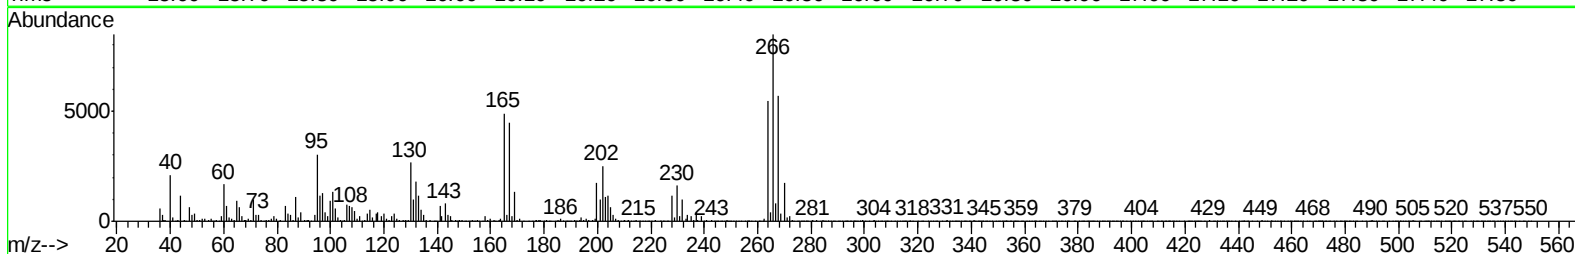


Data Path : Z:\HPCHEM1\BNA E\DATA\BE091415\
Data File : BE090809.D
Acq On : 14 Sep 2015 21:31
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 04:00:59 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 11:40:50 2015
Response via : Initial Calibration

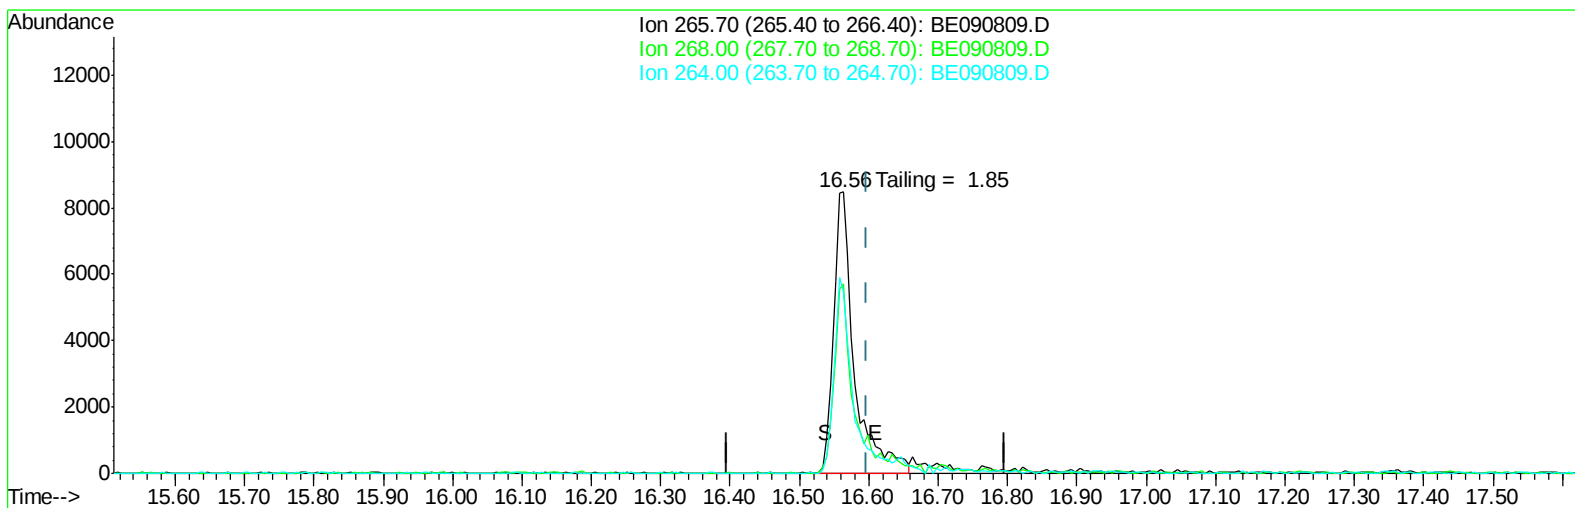

TIC: BE090809.D

(21) Pentachlorophenol

16.563min (-0.034) 56889.25ng

response 16759

Ion	Exp%	Act%
265.70	100	100
268.00	62.00	67.35
264.00	67.40	64.72
0.00	0.00	0.00