


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091415\
 Data File : BE090795.D
 Acq On : 14 Sep 2015 10:01
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 02 11:40:50 2015

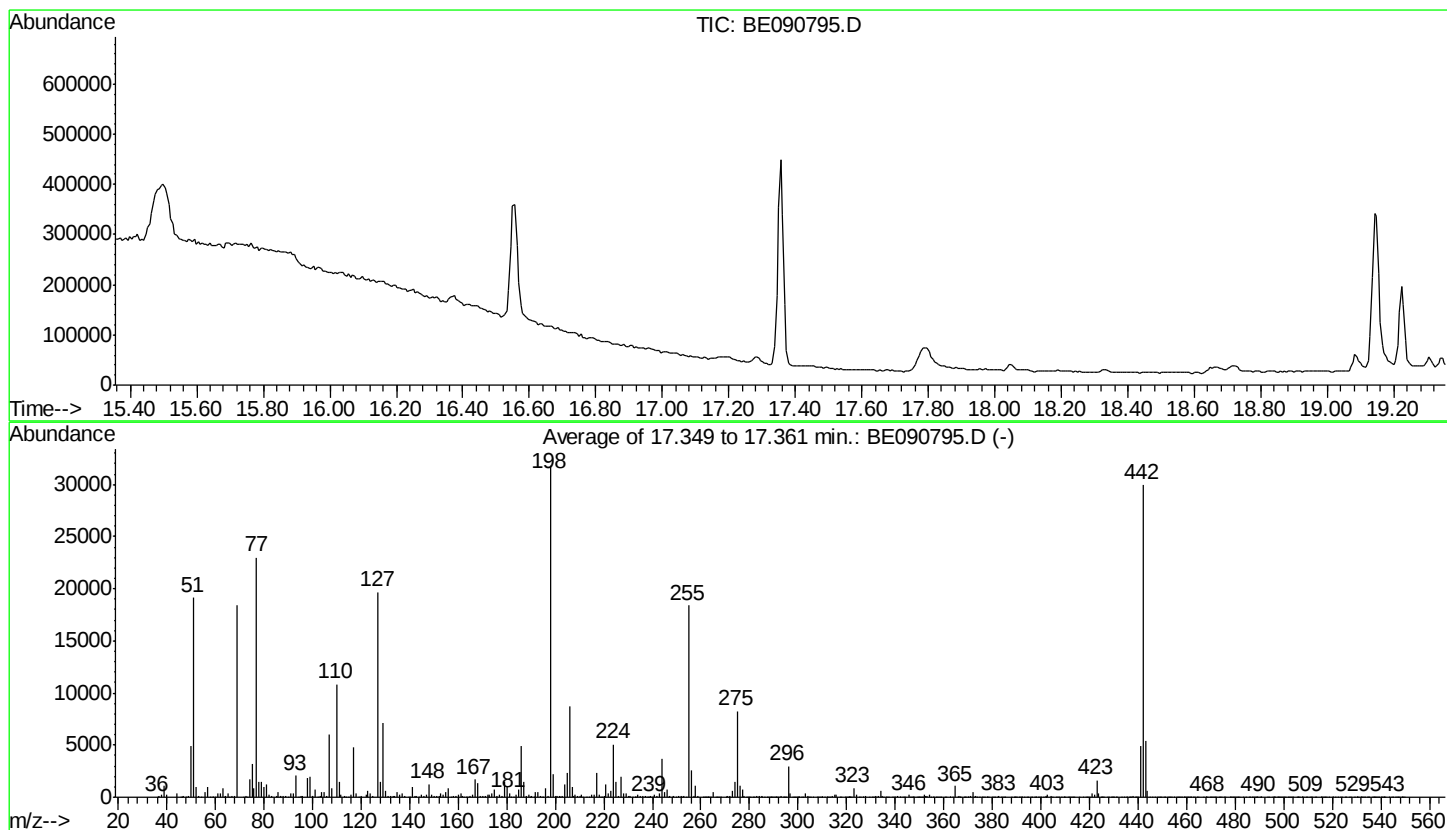

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.2	19142	PASS
68	69	0.00	2	0.8	146	PASS
69	198	0.00	100	57.9	18418	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	61.8	19667	PASS
197	198	0.00	2	0.4	122	PASS
198	198	100	100	100.0	31811	PASS
199	198	5	9	6.9	2203	PASS
275	198	10	60	25.9	8248	PASS
365	198	1	100	3.5	1098	PASS
441	442	0.01	24	16.5	4964	PASS
442	198	50	100	94.3	30008	PASS
443	442	15	24	18.1	5436	PASS