


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091415\
Data File : BE090809.D
Acq On : 14 Sep 2015 21:31
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 02 11:40:50 2015

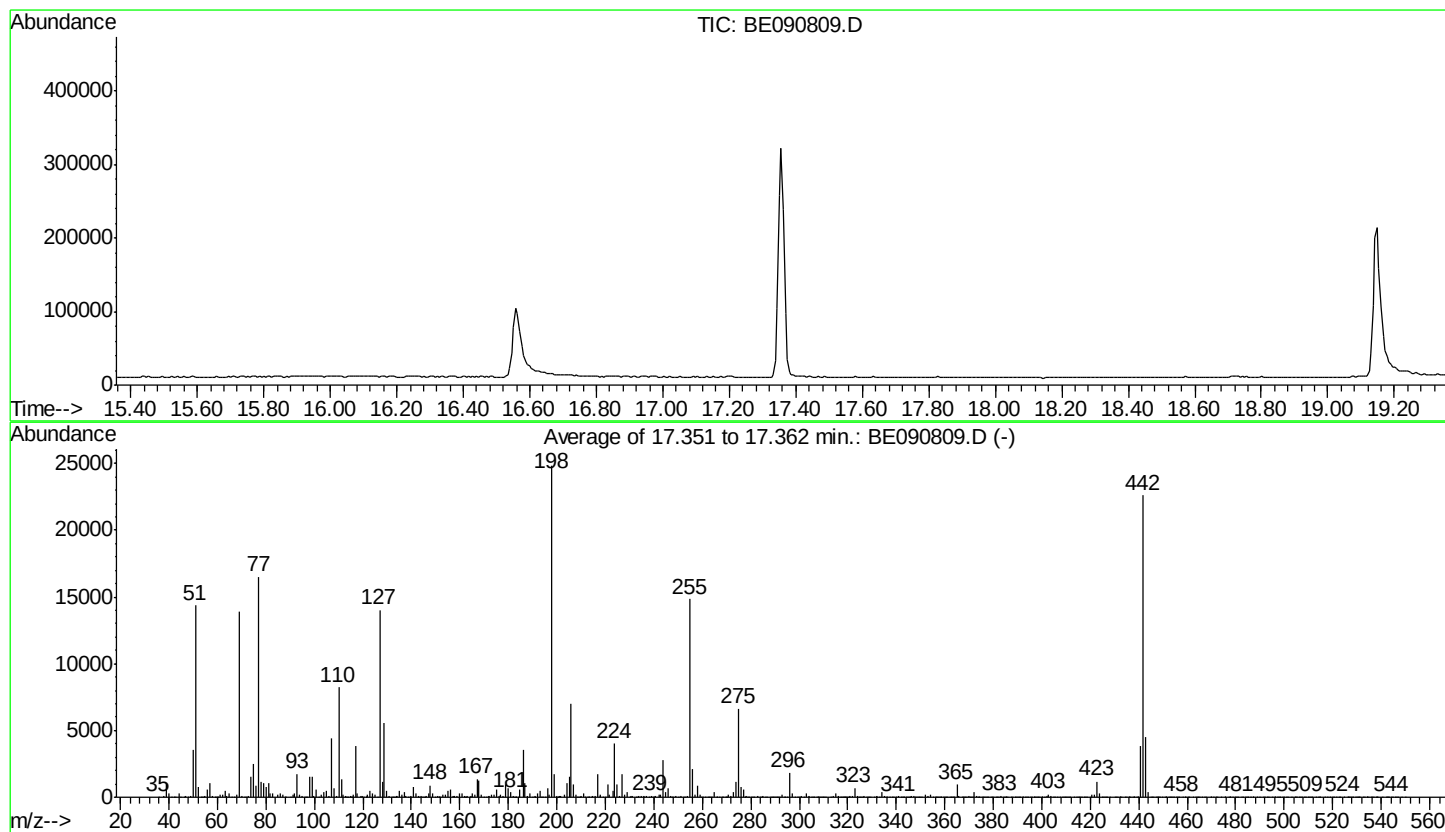

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.8	14354	PASS
68	69	0.00	2	1.1	153	PASS
69	198	0.00	100	55.9	13888	PASS
70	69	0.00	2	0.5	63	PASS
127	198	10	80	56.6	14050	PASS
197	198	0.00	2	0.9	221	PASS
198	198	100	100	100.0	24841	PASS
199	198	5	9	7.0	1728	PASS
275	198	10	60	26.7	6622	PASS
365	198	1	100	3.8	936	PASS
441	442	0.01	24	17.1	3869	PASS
442	198	50	100	91.0	22616	PASS
443	442	15	24	20.1	4556	PASS