
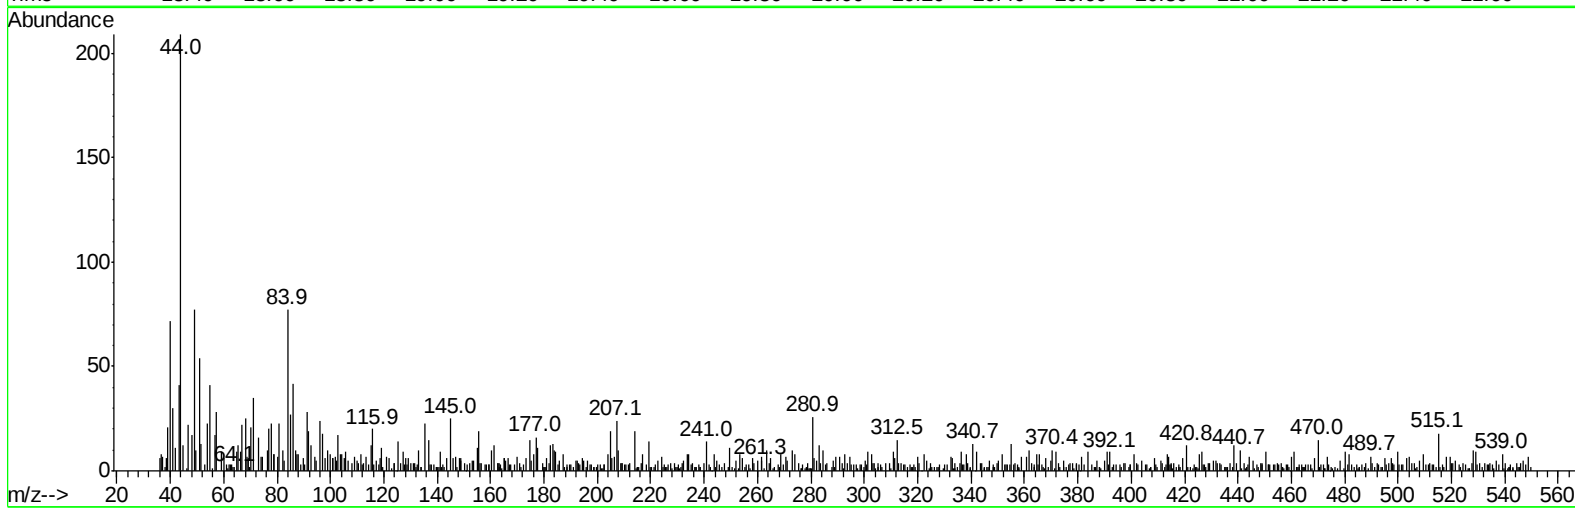


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE091417\
Data File : BE093997.D
Acq On : 14 Sep 2017 9:46
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 02:11:24 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

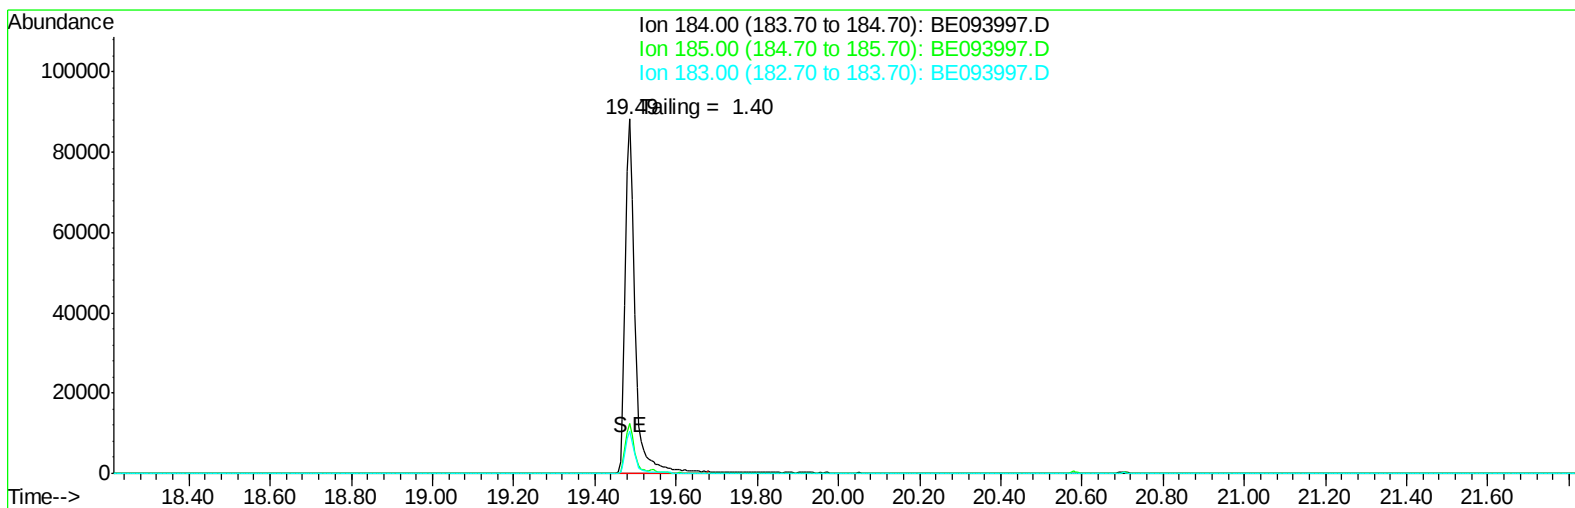

TIC: BE093997.D

(76) Benzidine



12.594min (+0.072) 316.34ng

response 14

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	42.11#
183.00	12.20	68.42#
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE091417\
Data File : BE093997.D
Acq On : 14 Sep 2017 9:46
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 02:11:24 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

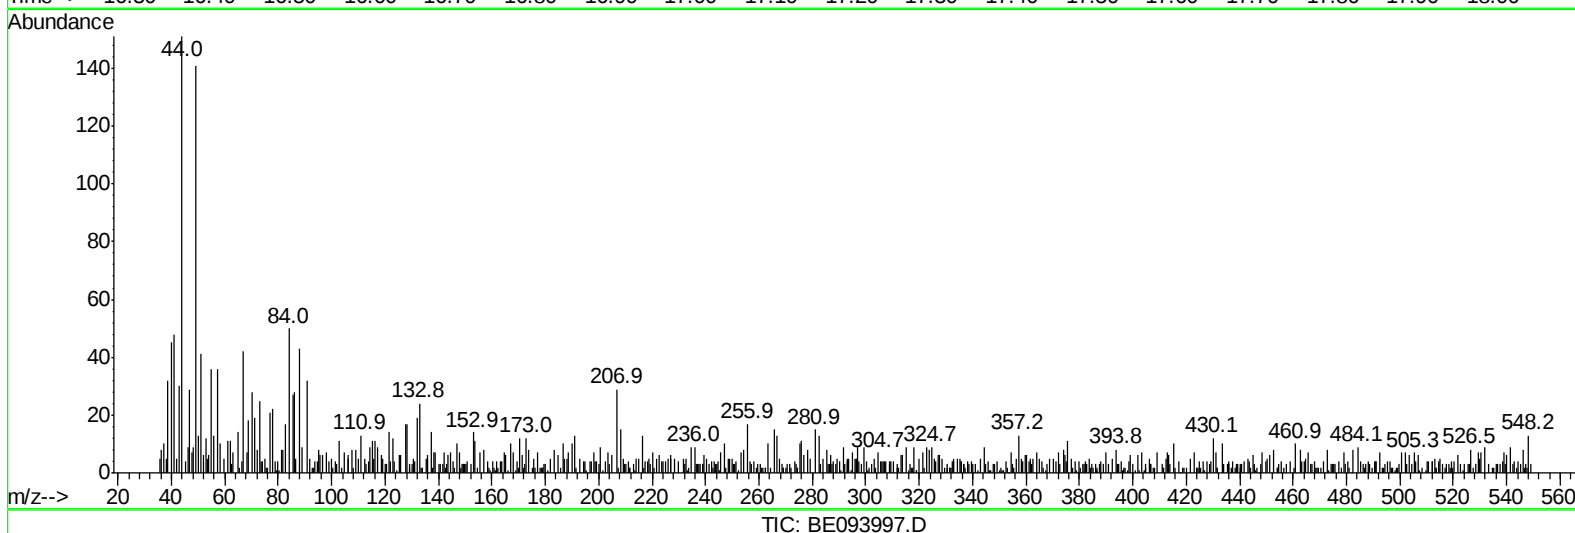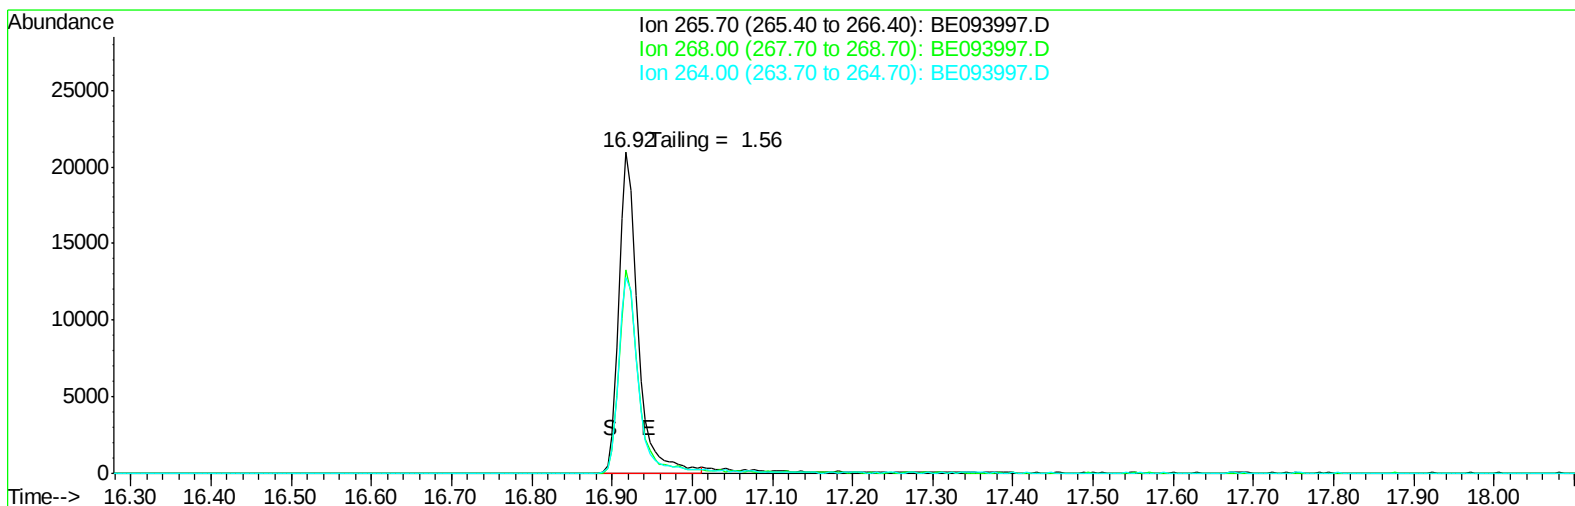

(69) Pentachlorophenol (C)

11.054min (+0.057) 183.43ng

response 14

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	20.00#
264.00	64.60	13.33#
0.00	0.00	0.00