

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE091417\
 Data File : BE094001.D
 Acq On : 14 Sep 2017 12:15
 Operator : SJ/JU
 Sample : I5189-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PR-MW-04-090817

Quant Time: Sep 15 01:20:57 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 05 13:34:56 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	2358	0.40	ng	0.00
7) Naphthalene-d8	10.72	136	11052	0.40	ng	0.02
13) Acenaphthene-d10	14.52	164	6609	0.40	ng	0.00
19) Phenanthrene-d10	17.27	188	14995	0.40	ng	0.00
27) Chrysene-d12	21.43	240	15496	0.40	ng	0.00
34) Perylene-d12	23.94	264	11678	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.53	112	1048	0.14	ng	0.00
5) Phenol-d6	7.13	99	767	0.07	ng	0.01
8) Nitrobenzene-d5	9.08	82	3163	0.34	ng	0.00
11) 2-Methylnaphthalene-d10	12.31	152	5878	0.33	ng	0.01
14) 2,4,6-Tribromophenol	16.03	330	608	0.30	ng	0.00
15) 2-Fluorobiphenyl	13.18	172	9263	0.35	ng	0.02
25) Fluoranthene-d10	19.28	212	62441	0.28	ng	0.00
29) Terphenyl-d14	19.87	244	12528	0.44	ng	0.00
Target Compounds						
32) Bis(2-ethylhexyl)phthalate	21.30	149	2607	0.023	ng	Qvalue # 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE091417\
Data File : BE094001.D
Acq On : 14 Sep 2017 12:15
Operator : SJ/JU
Sample : I5189-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PR-MW-04-090817

Quant Time: Sep 15 01:20:57 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 05 13:34:56 2017
Response via : Initial Calibration

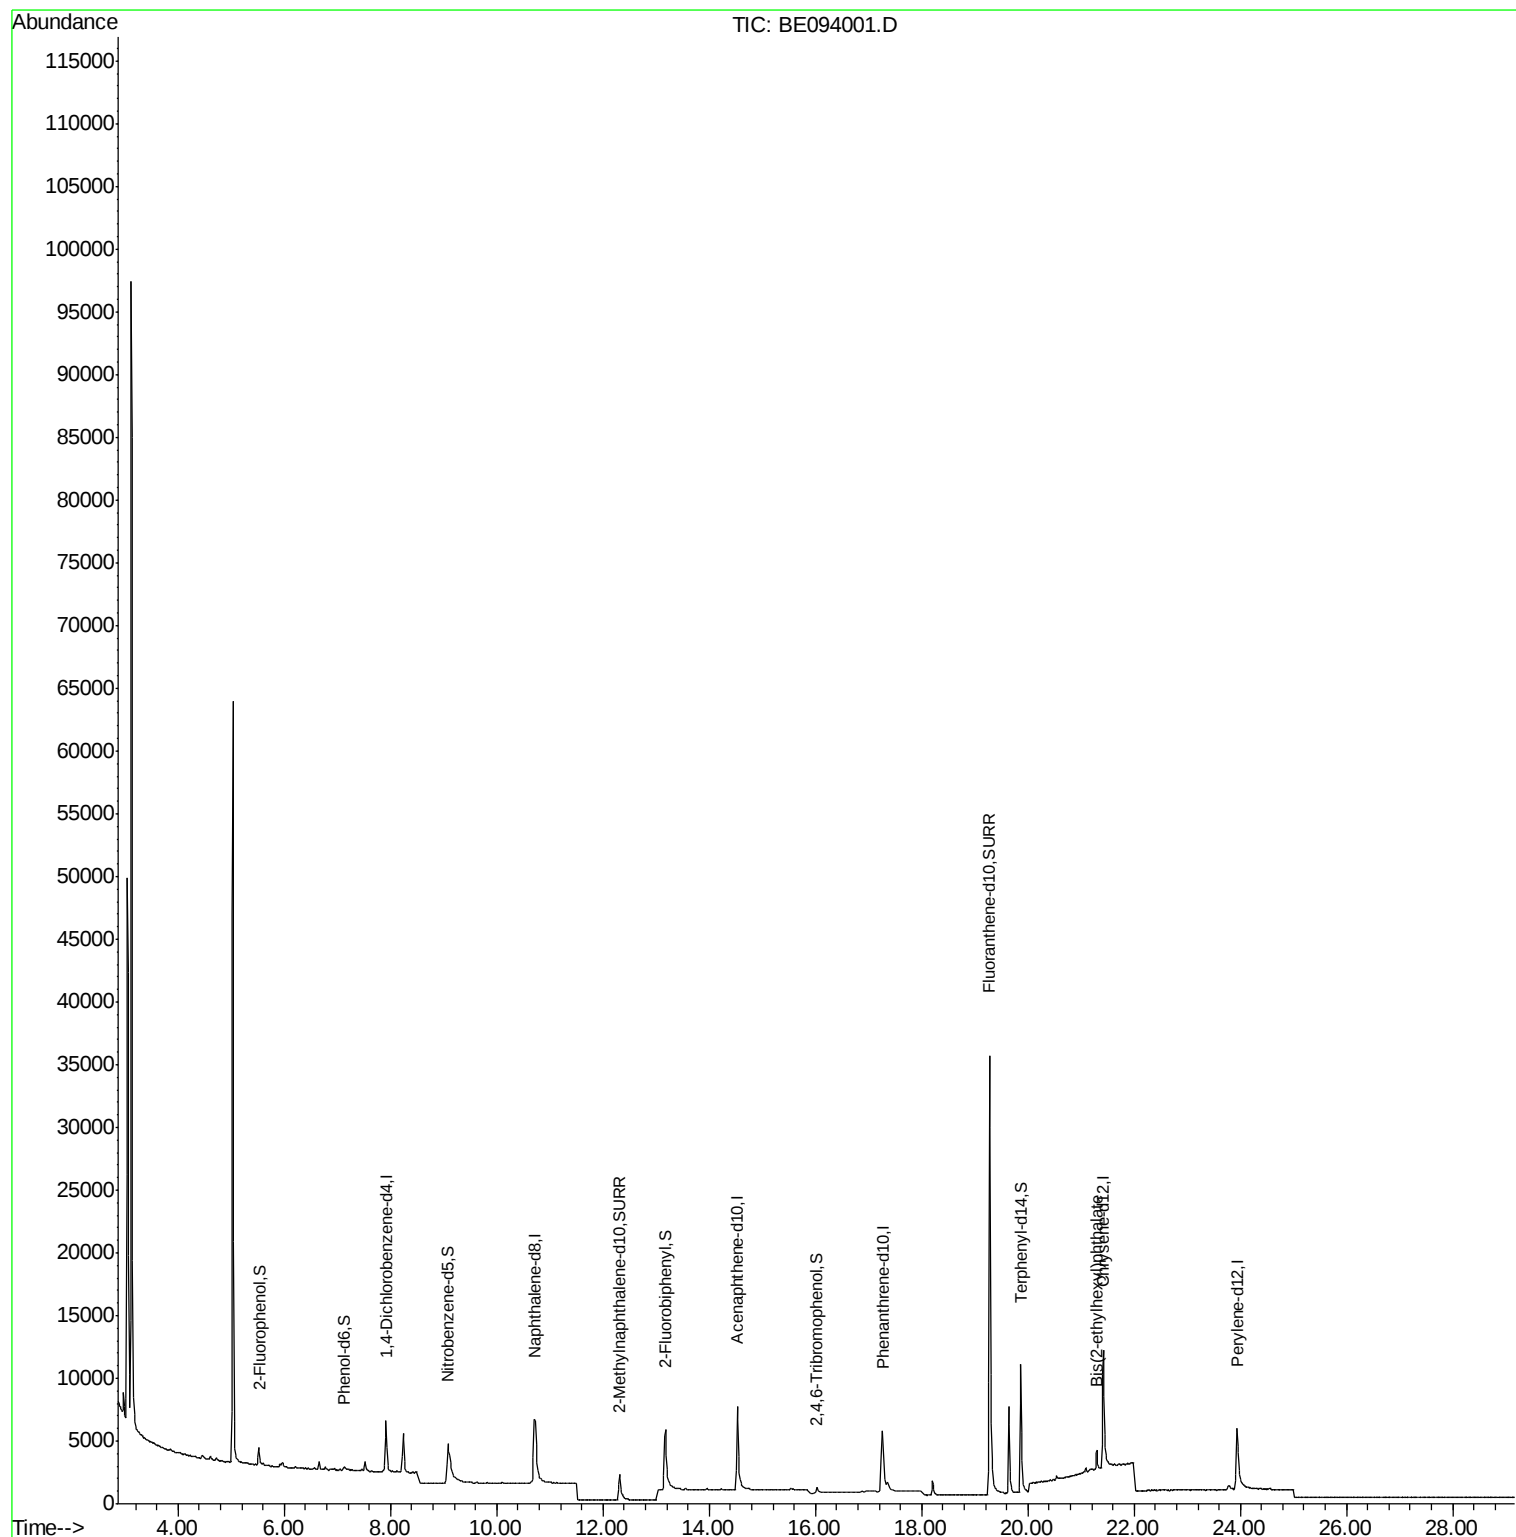



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.92 min Scan# 402

Delta R.T. -0.00 min

Lab File: BE094001.D

Acq: 14 Sep 2017 12:15

Instrument :

BNA_E

ClientSampleId :

PR-MW-04-090817


Tot Ion:152 Resp: 2358

Ion Ratio Lower Upper

152 100

150 153.2 121.8 182.6




115 66.5 52.6 79.0

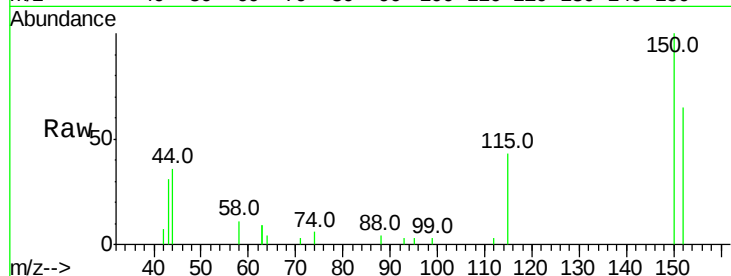

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

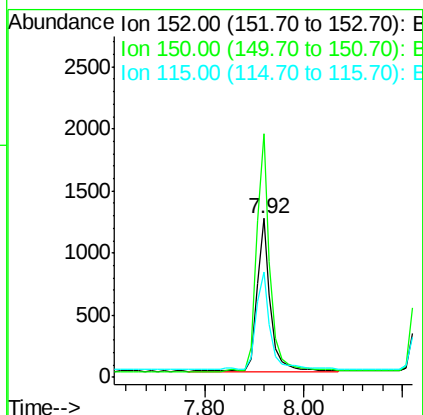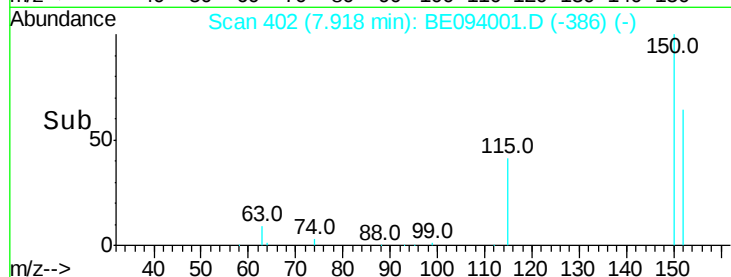

#4

2-Fluorophenol

Concen: 0.137 ng

RT: 5.53 min Scan# 212

Delta R.T. -0.00 min

Lab File: BE094001.D

Acq: 14 Sep 2017 12:15


Tgt Ion:112 Resp: 1048

Ion Ratio Lower Upper

112 100

64 71.4 57.7 86.5



63 144.2 116.0 174.0




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

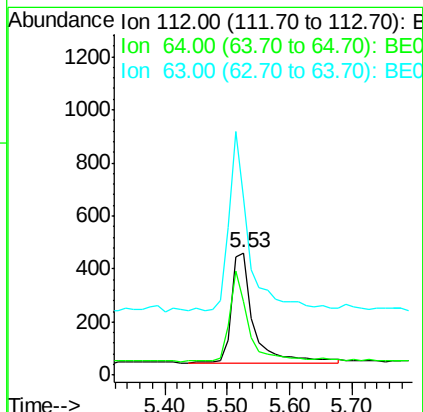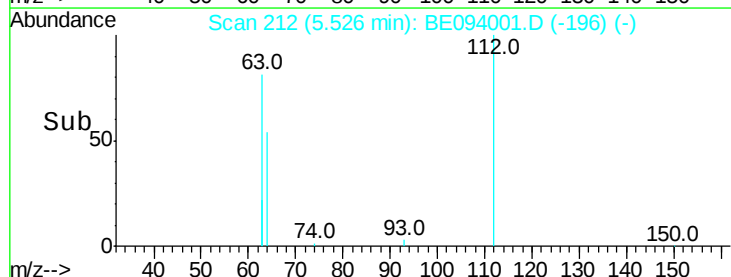



#5

Phenol-d6

Concen: 0.067 ng

RT: 7.13 min Scan# 339

Delta R.T. 0.01 min

Lab File: BE094001.D

Acq: 14 Sep 2017 12:15

Instrument :

BNA_E

ClientSampleId :

PR-MW-04-090817





Tot Ion: 99 Resp: 767

Ion Ratio Lower Upper

99 100

42 18.8 17.1 25.7

71 25.4 26.6 39.8#

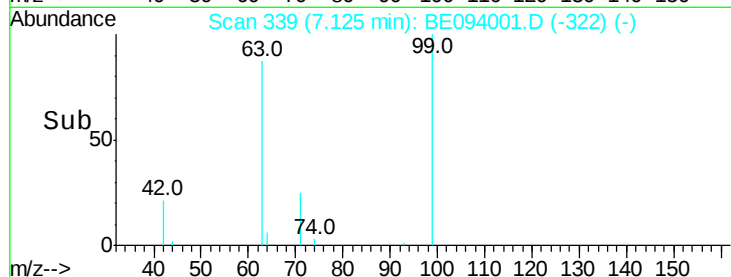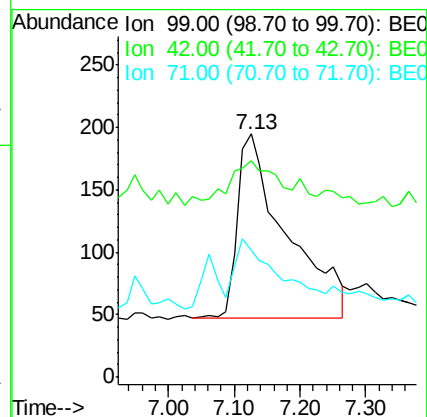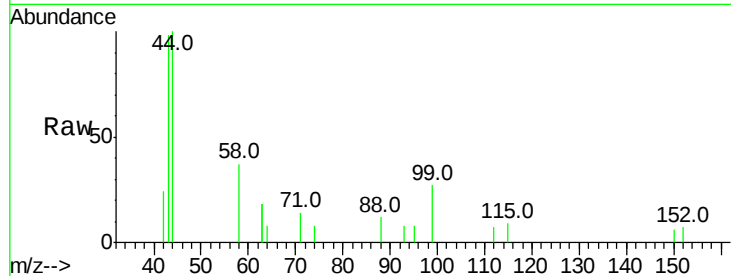

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.72 min Scan# 578

Delta R.T. 0.02 min

Lab File: BE094001.D

Acq: 14 Sep 2017 12:15

Tgt Ion: 136 Resp: 11052




Ion Ratio Lower Upper


136 100

137 12.5 9.2 13.8

54 40.5 21.9 32.9#

68 7.9 4.6 7.0#

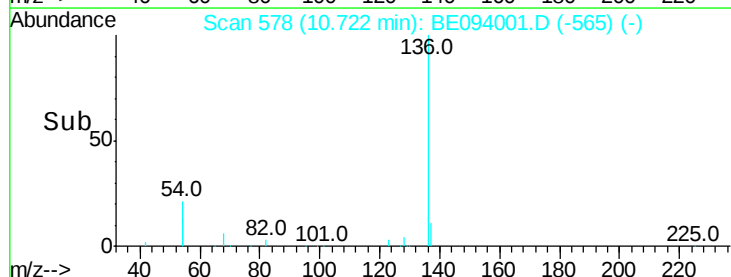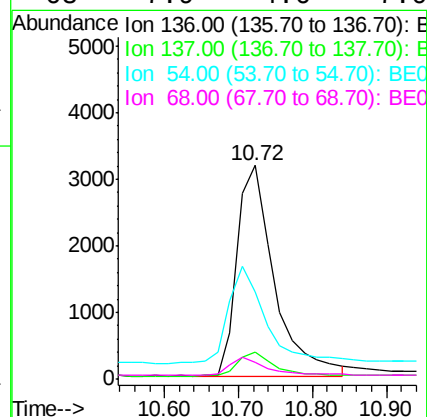



#8

Nitrobenzene-d5

Concen: 0.338 ng

RT: 9.08 min Scan# 480

Delta R.T. -0.00 min

Lab File: BE094001.D

Acq: 14 Sep 2017 12:15

Instrument :

BNA_E

ClientSampleId :

PR-MW-04-090817


Tot Ion: 82 Resp: 3163

Ion Ratio Lower Upper

82 100

128 145.3 91.4 137.0#




54 233.7 197.8 296.8

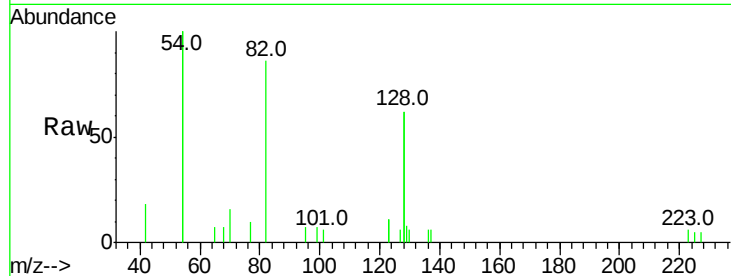

Abundance Ion 82.00 (81.70 to 82.70): BE093930.D (-477) (-)

Ion 128.00 (127.70 to 128.70): BE093930.D (-477) (-)

Ion 54.00 (53.70 to 54.70): BE093930.D (-477) (-)

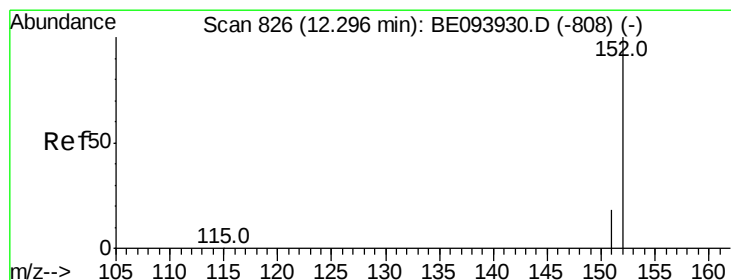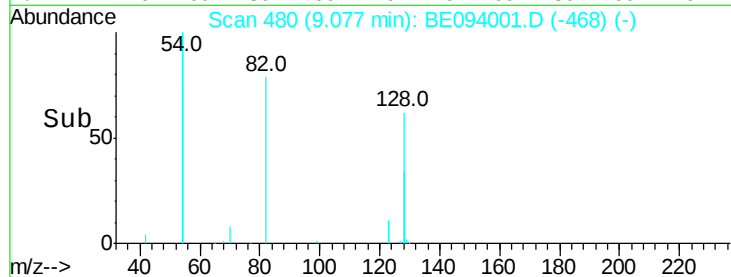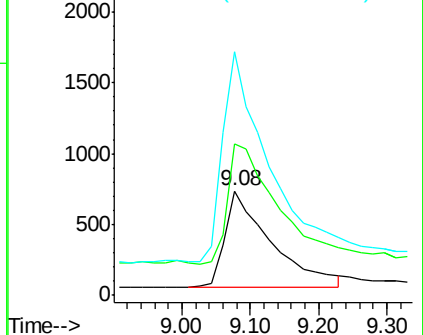

#11

2-Methylnaphthalene-d10

Concen: 0.332 ng

RT: 12.31 min Scan# 830

Delta R.T. 0.01 min

Lab File: BE094001.D


Acq: 14 Sep 2017 12:15

Tgt Ion: 152 Resp: 5878

Ion Ratio Lower Upper



152 100


151 18.5 15.4 23.0



Abundance Ion 152.00 (151.70 to 152.70): BE093930.D (-808) (-)

Ion 151.00 (150.70 to 151.70): BE093930.D (-808) (-)



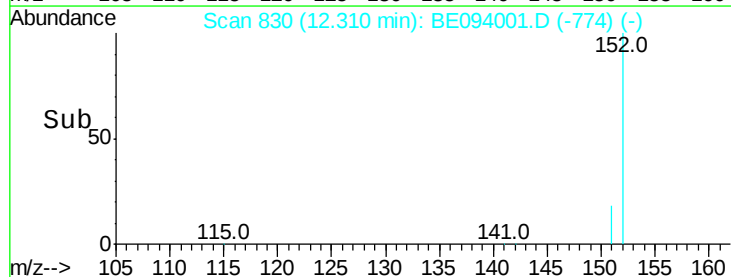
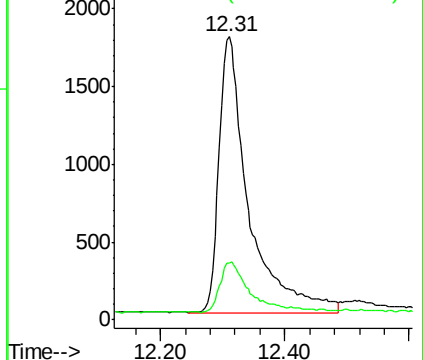




#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.52 min Scan# 1112
 Delta R.T. 0.00 min
 Lab File: BE094001.D
 Acq: 14 Sep 2017 12:15




Instrument :
 BNA_E
 ClientSampleId :
 PR-MW-04-090817


Tot Ion:164 Resp: 6609
 Ion Ratio Lower Upper
 164 100
 162 107.4 80.8 121.2
 160 50.4 37.0 55.4

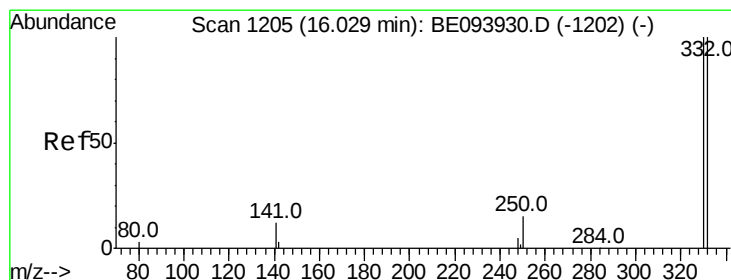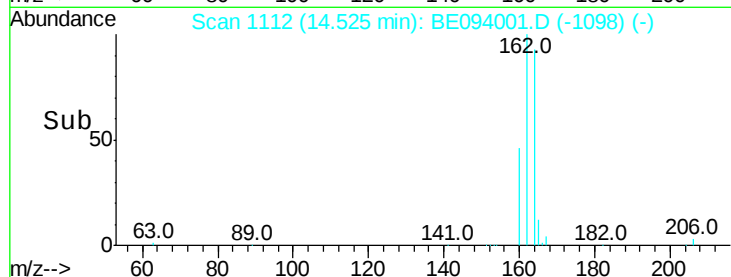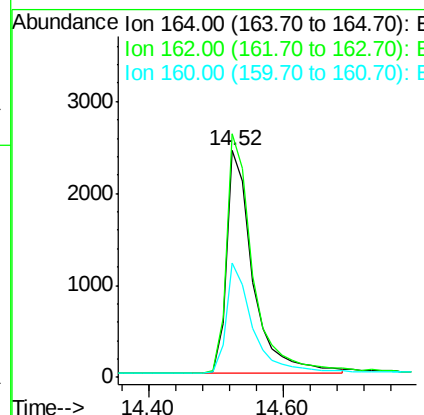

#14
 2,4,6-Tribromophenol
 Concen: 0.297 ng
 RT: 16.03 min Scan# 1206
 Delta R.T. 0.00 min
 Lab File: BE094001.D
 Acq: 14 Sep 2017 12:15

Tgt Ion:330 Resp: 608
 Ion Ratio Lower Upper
 330 100
 332 92.6 76.9 115.3
 141 0.0 0.0 0.0

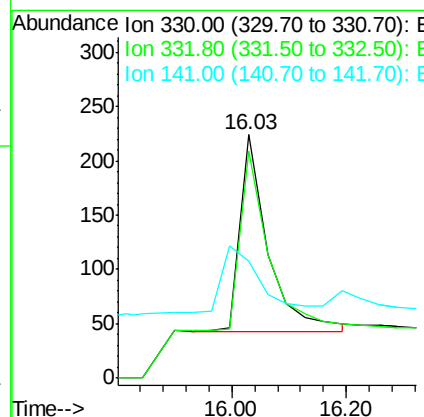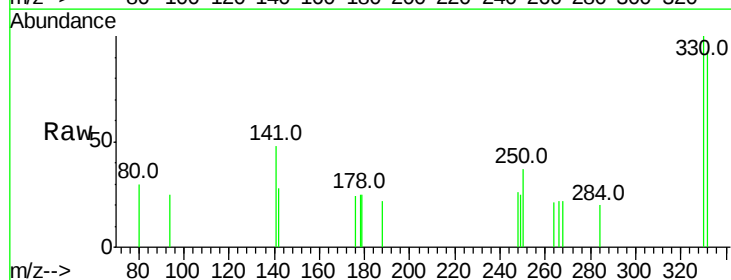

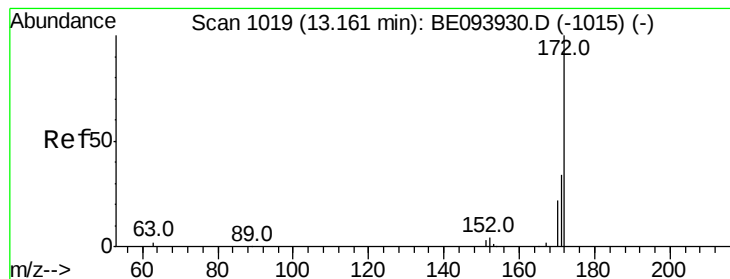

#15

2-Fluorobiphenyl

Concen: 0.354 ng

RT: 13.18 min Scan# 1021

Delta R.T. 0.02 min

Lab File: BE094001.D

Acq: 14 Sep 2017 12:15

Instrument :

BNA_E

ClientSampleId :

PR-MW-04-090817


Tot Ion:172 Resp: 9263

Ion Ratio Lower Upper

172 100

171 35.7 26.9 40.3




170 22.9 17.3 25.9

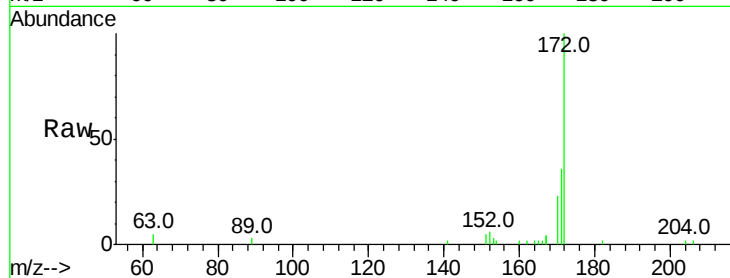

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

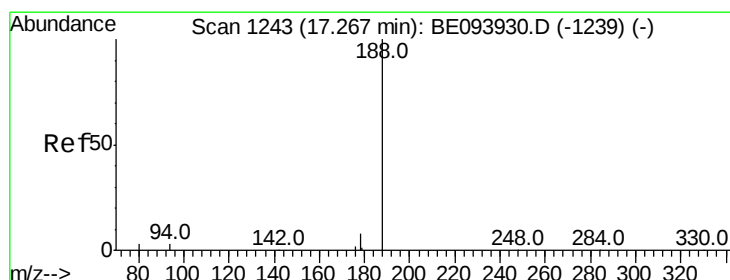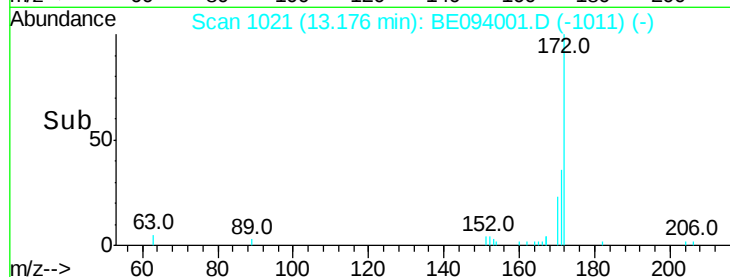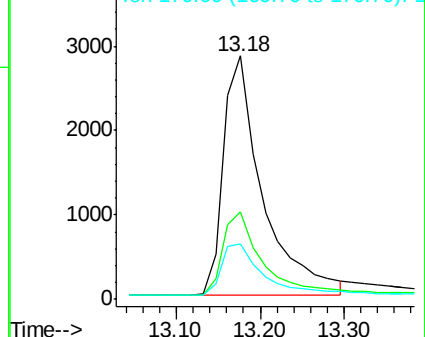

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.27 min Scan# 1244

Delta R.T. 0.00 min

Lab File: BE094001.D

Acq: 14 Sep 2017 12:15


Tgt Ion:188 Resp: 14995

Ion Ratio Lower Upper

188 100

94 6.3 16.1 24.1#



80 6.5 18.2 27.2#

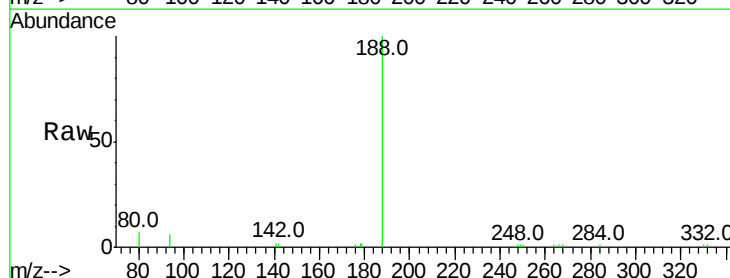


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0



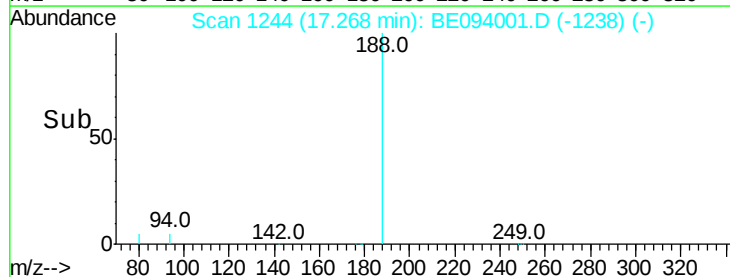
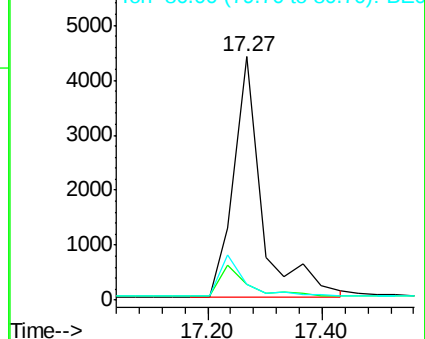




#25
 Fluoranthene-d10
 Concen: 0.279 ng
 RT: 19.28 min Scan# 1433
 Delta R.T. -0.00 min
 Lab File: BE094001.D
 Acq: 14 Sep 2017 12:15




Instrument :
 BNA_E
 ClientSampleId :
 PR-MW-04-090817


Tot Ion:212 Resp: 62441
 Ion Ratio Lower Upper
 212 100
 106 3.4 2.7 4.1
 104 2.0 1.6 2.4

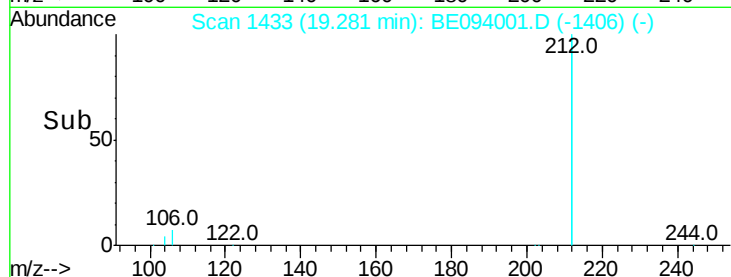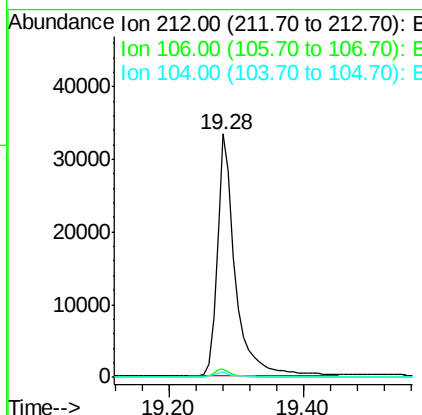

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.43 min Scan# 1656
 Delta R.T. -0.00 min
 Lab File: BE094001.D
 Acq: 14 Sep 2017 12:15

Tgt Ion:240 Resp: 15496
 Ion Ratio Lower Upper
 240 100
 120 10.4 8.7 13.1
 236 26.5 21.3 31.9

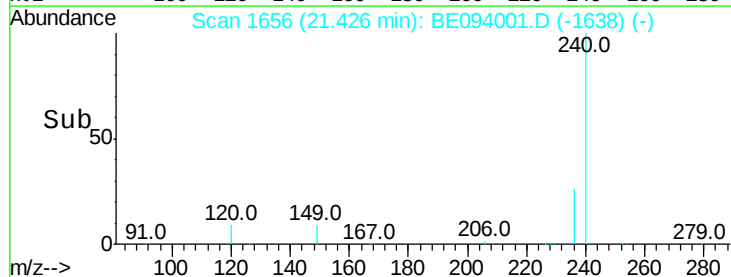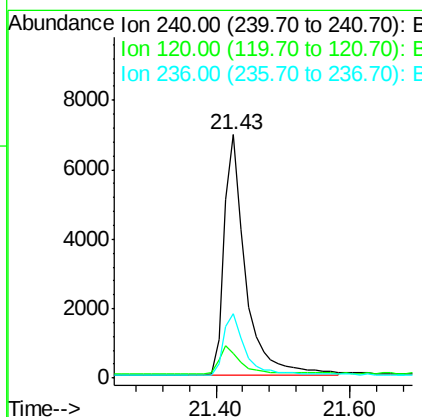



#29

Terphenyl-d14

Concen: 0.439 ng

RT: 19.87 min Scan# 1512

Delta R.T. -0.01 min

Lab File: BE094001.D

Acq: 14 Sep 2017 12:15

Instrument :

BNA_E

ClientSampleId :

PR-MW-04-090817


Tot Ion:244 Resp: 12528

Ion Ratio Lower Upper

244 100

212 35.8 28.3 42.5




122 13.2 9.4 14.0



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

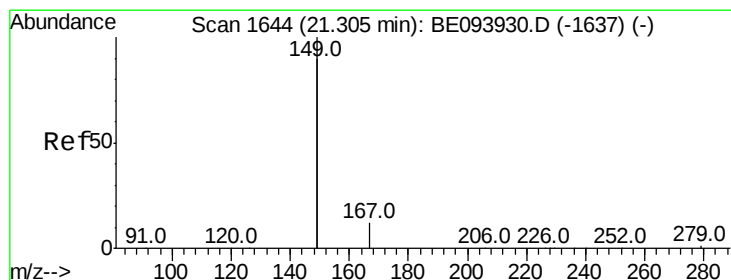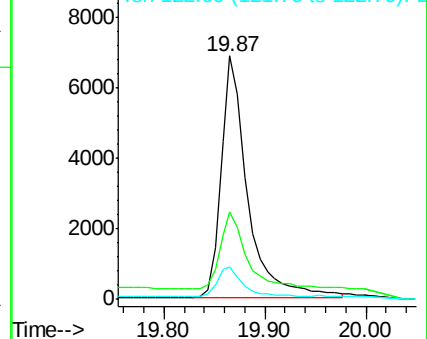

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.023 ng

RT: 21.30 min Scan# 1645

Delta R.T. -0.00 min

Lab File: BE094001.D

Acq: 14 Sep 2017 12:15


Tgt Ion:149 Resp: 2607

Ion Ratio Lower Upper

149 100

167 6.6 5.4 8.0



279 1.4 0.7 1.1#



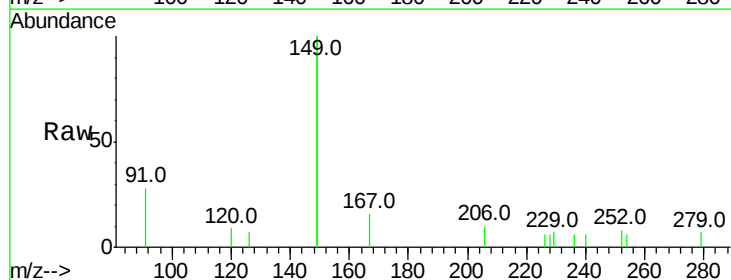


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

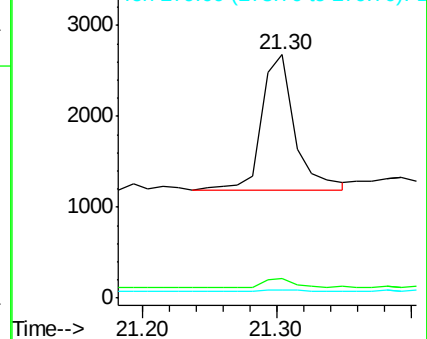



#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.94 min Scan# 2129

Delta R.T. 0.00 min

Lab File: BE094001.D

Acq: 14 Sep 2017 12:15

Instrument :

BNA_E

ClientSampleId :

PR-MW-04-090817

Tot Ion: 264 Resp: 11678

Ion Ratio Lower Upper

264 100

260 26.0 20.0 30.0

265 34.1 24.0 36.0

