


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE091417\
 Data File : BE093997.D
 Acq On : 14 Sep 2017 9:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 13:34:56 2017

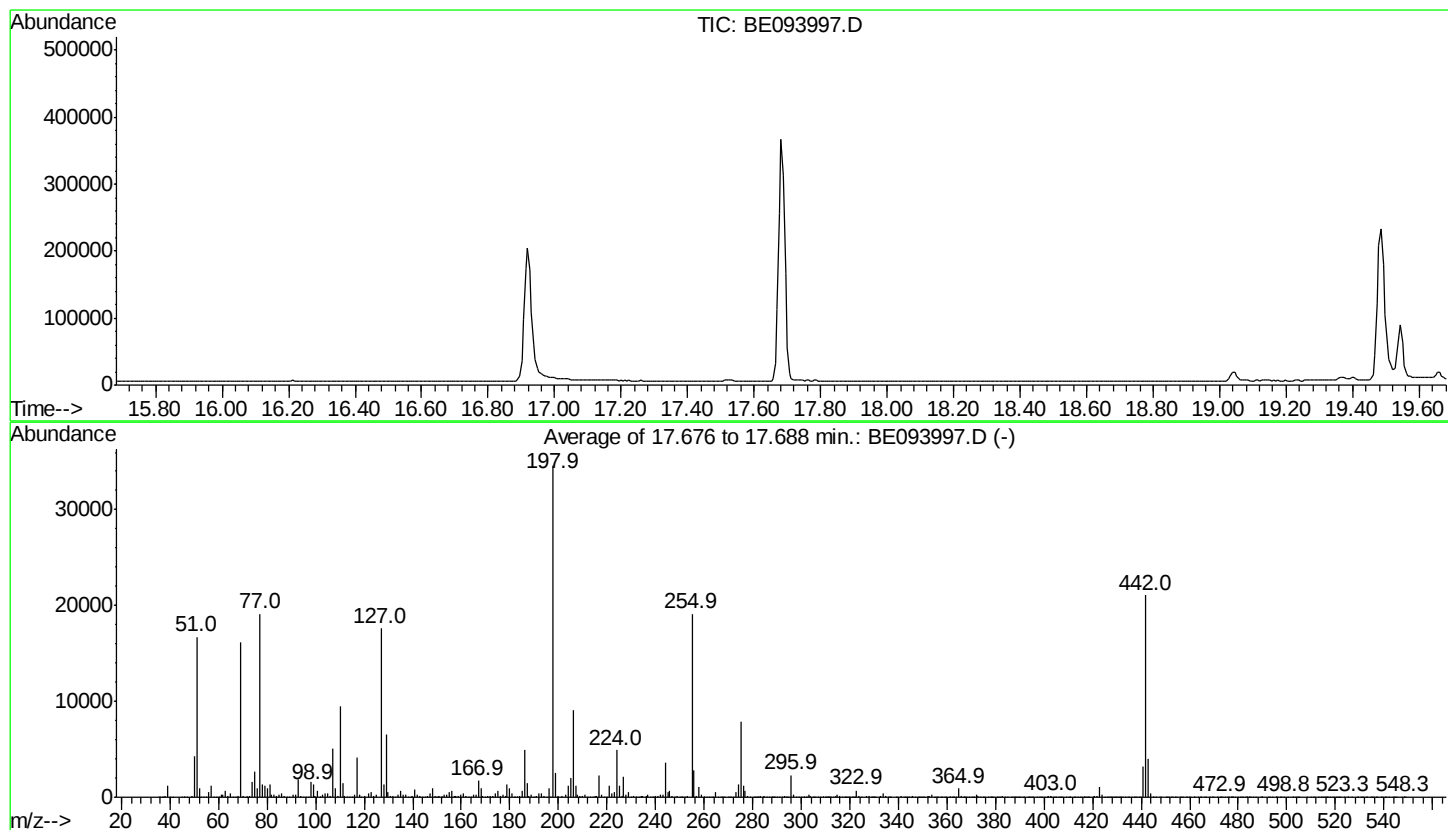

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	16749	PASS
68	69	0.00	2	0.5	75	PASS
69	198	0.00	100	46.6	16140	PASS
70	69	0.00	2	0.5	77	PASS
127	198	10	80	50.9	17618	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34601	PASS
199	198	5	9	7.3	2532	PASS
275	198	10	60	23.0	7950	PASS
365	198	1	100	2.5	876	PASS
441	442	0.01	24	15.0	3162	PASS
442	198	50	100	60.9	21082	PASS
443	442	15	24	19.0	4011	PASS