
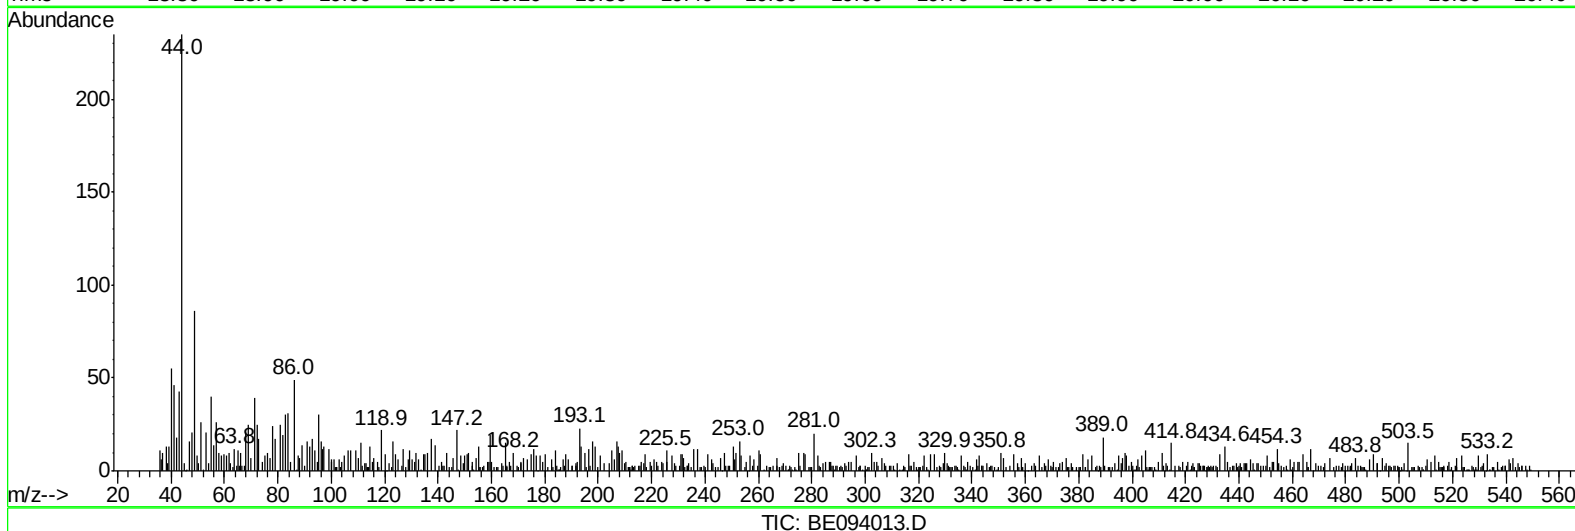


Data Path : Z:\HPCHEM1\BNA E\DATA\BE091517\
Data File : BE094013.D
Acq On : 15 Sep 2017 9:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 00:59:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

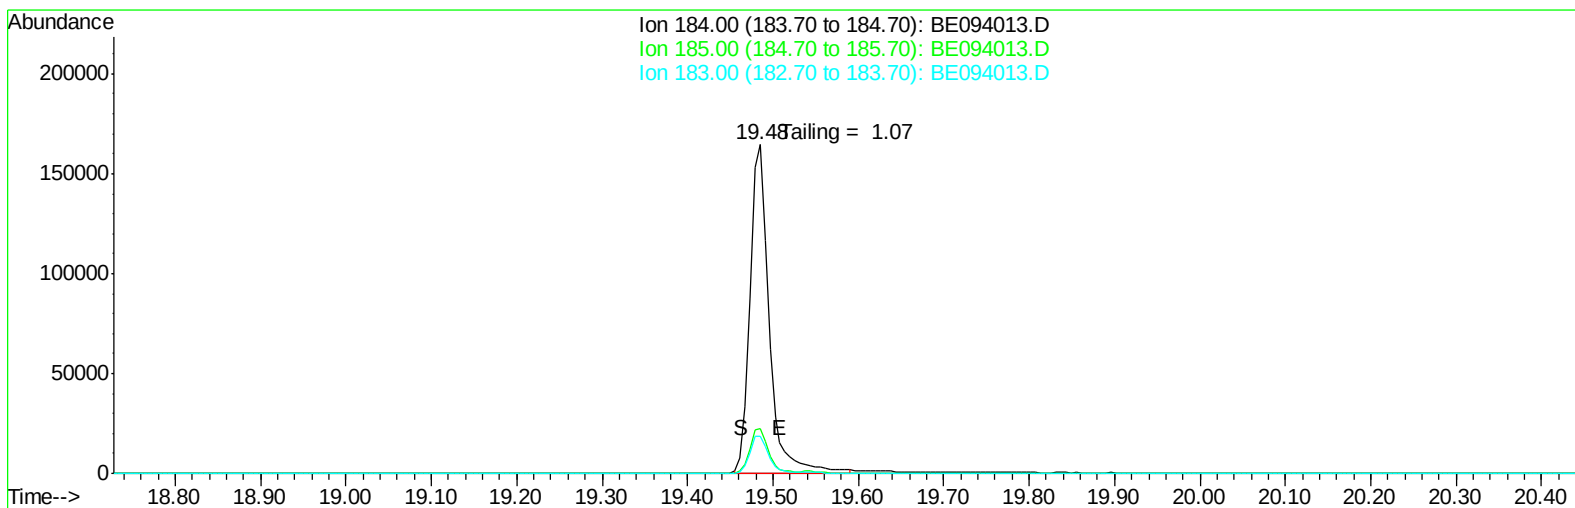

(76) Benzidine



12.687min (+0.166) 30.13ng

response 8

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	21.43
183.00	12.20	14.29
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE091517\
Data File : BE094013.D
Acq On : 15 Sep 2017 9:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 00:59:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

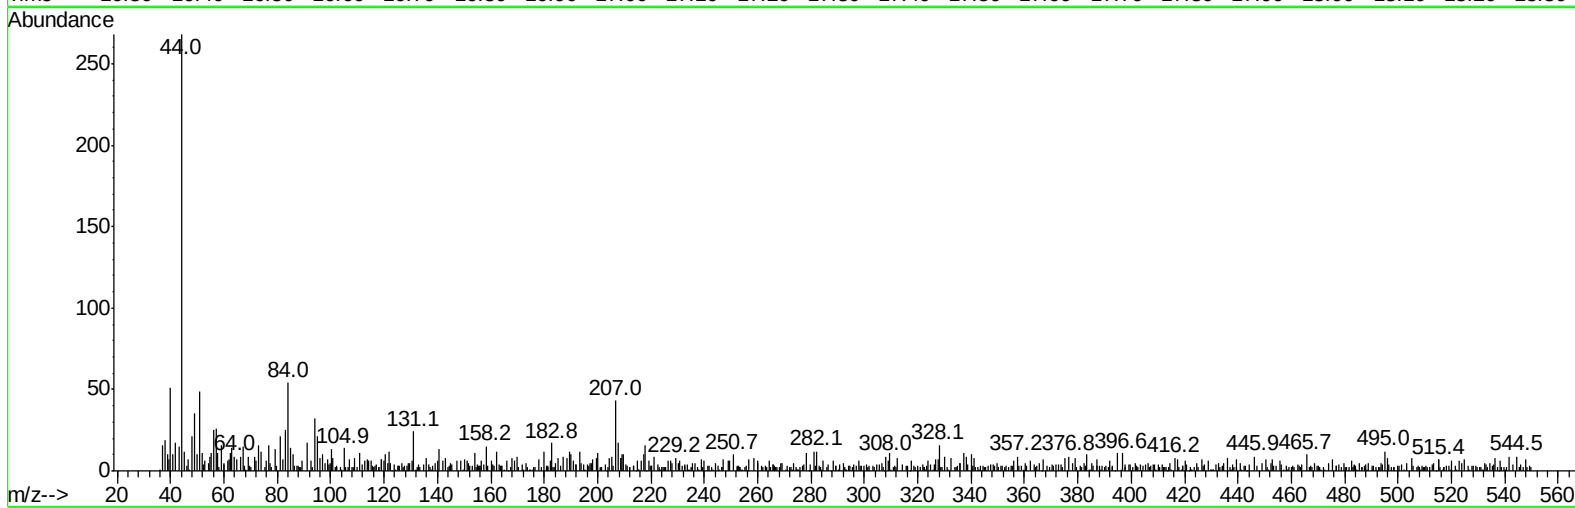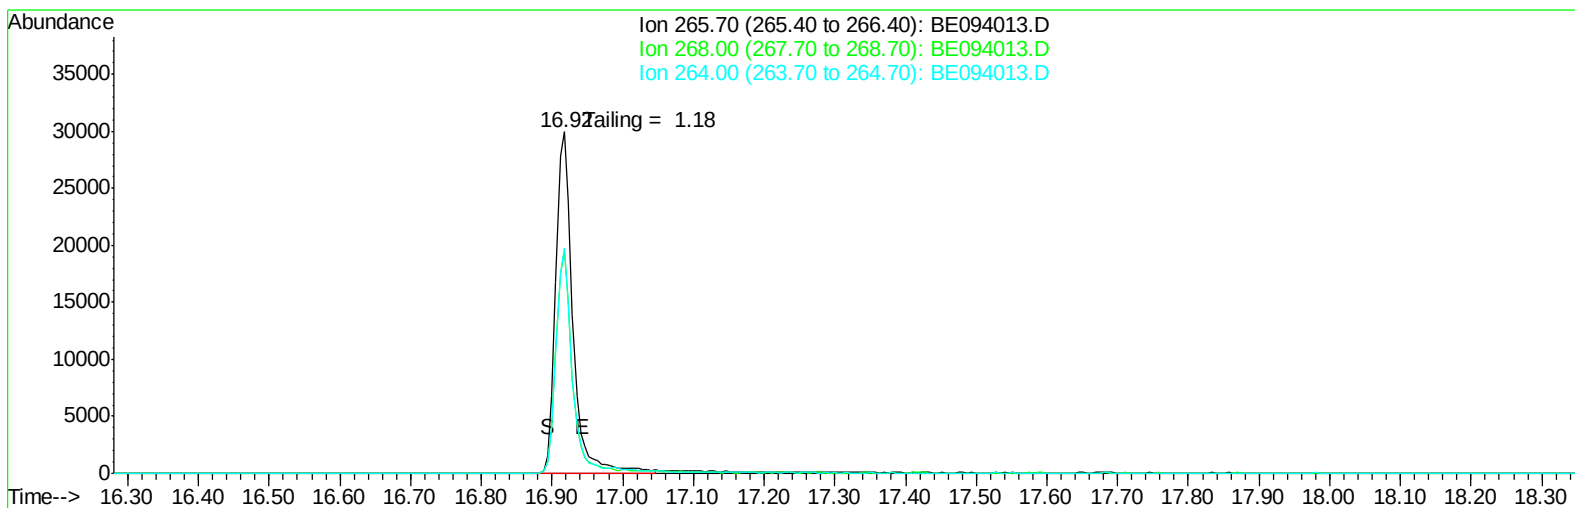

TIC: BE094013.D

(69) Pentachlorophenol (C)

11.236min (+0.239) 242.68ng

response 11

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.64
264.00	64.60	54.55
0.00	0.00	0.00