


Data Path : Z:\HPCHEM1\BNA E\DATA\BE091615\
Data File : BE090841.D
Acq On : 16 Sep 2015 10:56
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 02 11:40:50 2015

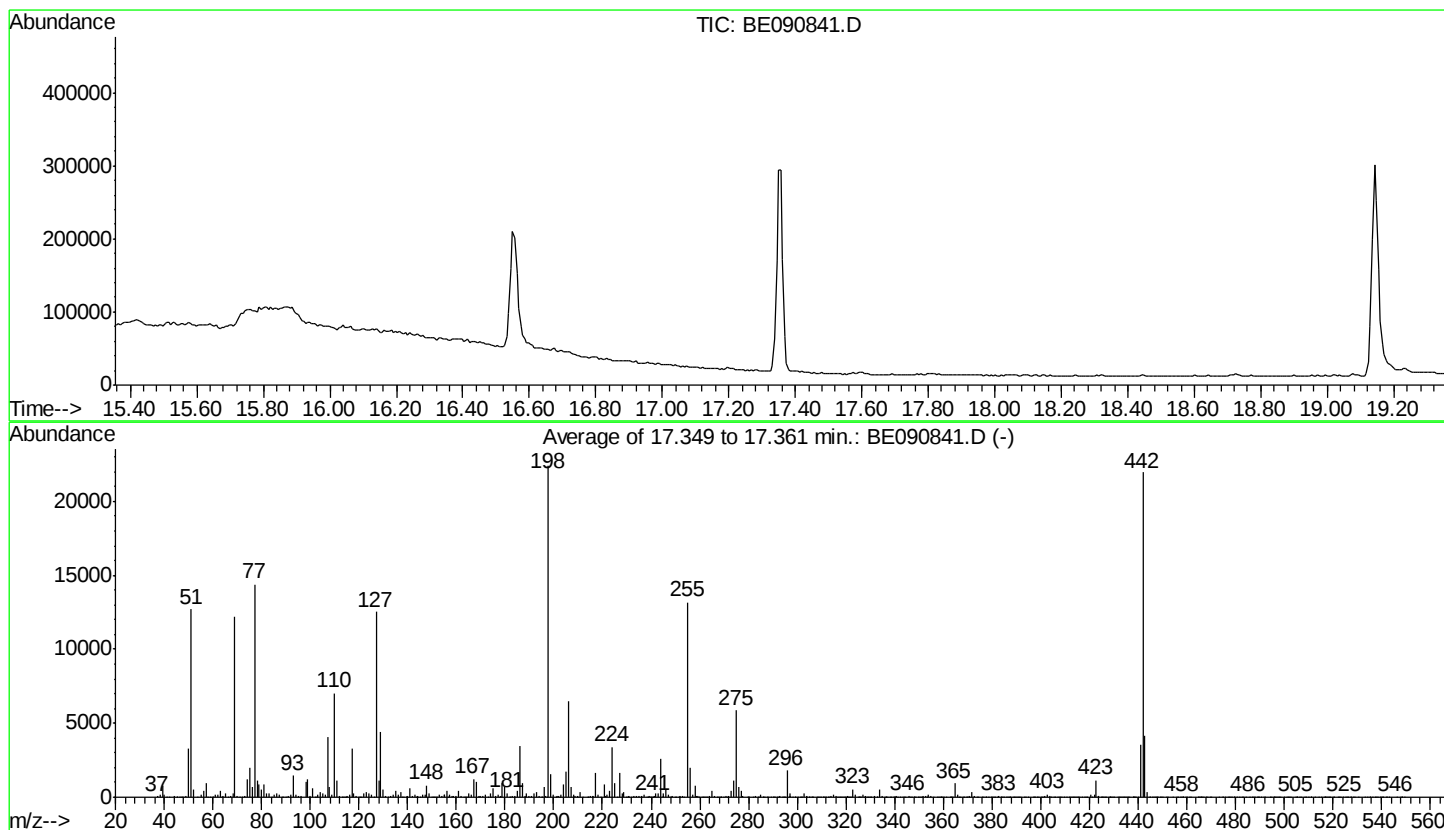

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.6	12685	PASS
68	69	0.00	2	1.8	220	PASS
69	198	0.00	100	54.5	12207	PASS
70	69	0.00	2	0.6	77	PASS
127	198	10	80	56.0	12545	PASS
197	198	0.00	2	0.1	21	PASS
198	198	100	100	100.0	22416	PASS
199	198	5	9	6.8	1523	PASS
275	198	10	60	26.1	5849	PASS
365	198	1	100	4.1	921	PASS
441	442	0.01	24	16.2	3574	PASS
442	198	50	100	98.1	21994	PASS
443	442	15	24	18.7	4117	PASS