


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091616\
Data File : BE092383.D
Acq On : 16 Sep 2016 8:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090216.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 02 19:34:51 2016

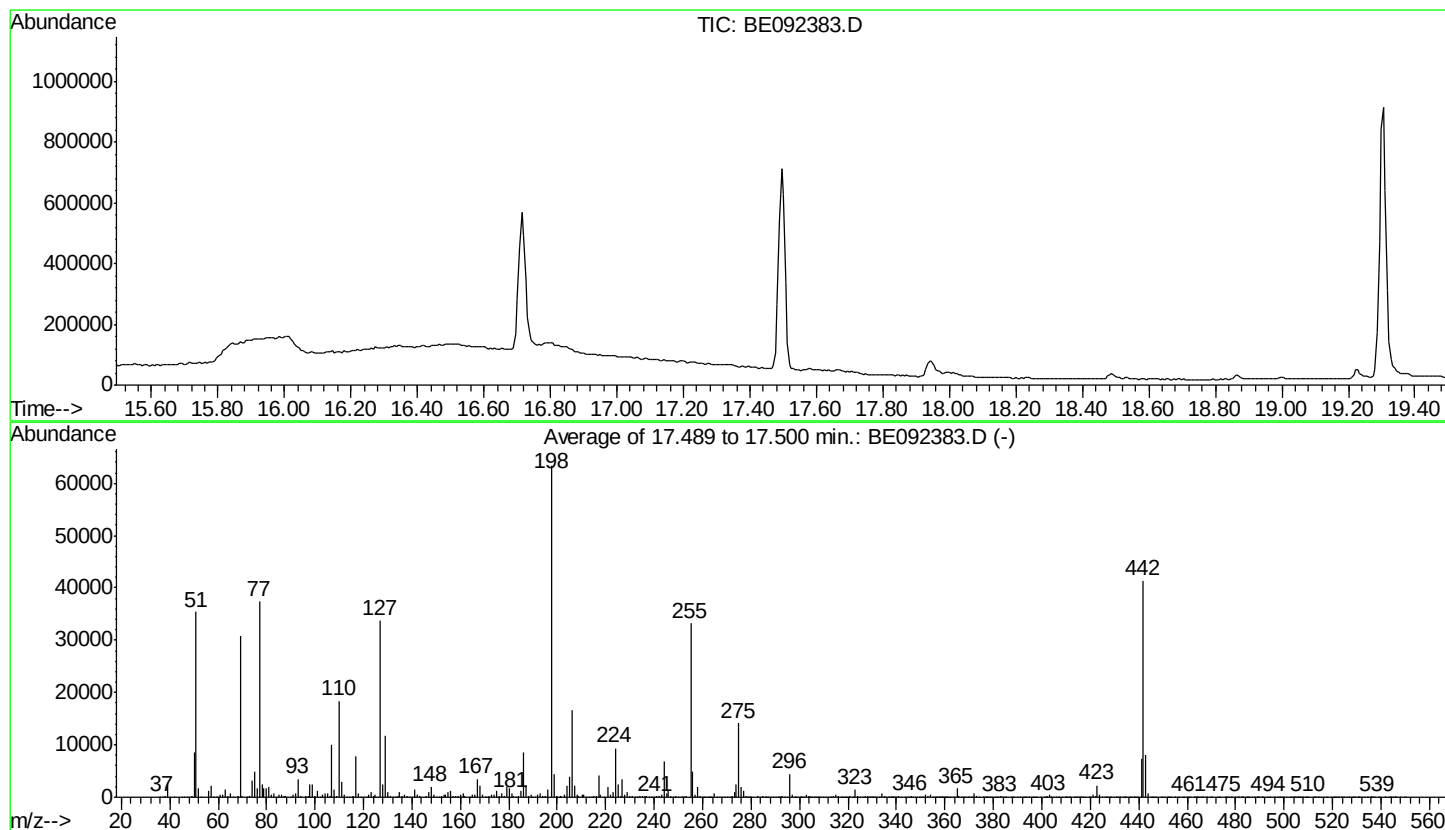

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.9	35398	PASS
68	69	0.00	2	1.2	369	PASS
69	198	0.00	100	48.6	30799	PASS
70	69	0.00	2	0.8	243	PASS
127	198	10	80	53.2	33723	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63354	PASS
199	198	5	9	7.1	4483	PASS
275	198	10	60	22.4	14177	PASS
365	198	1	100	2.6	1671	PASS
441	442	0.01	24	17.8	7389	PASS
442	198	50	100	65.4	41415	PASS
443	442	15	24	19.8	8180	PASS