
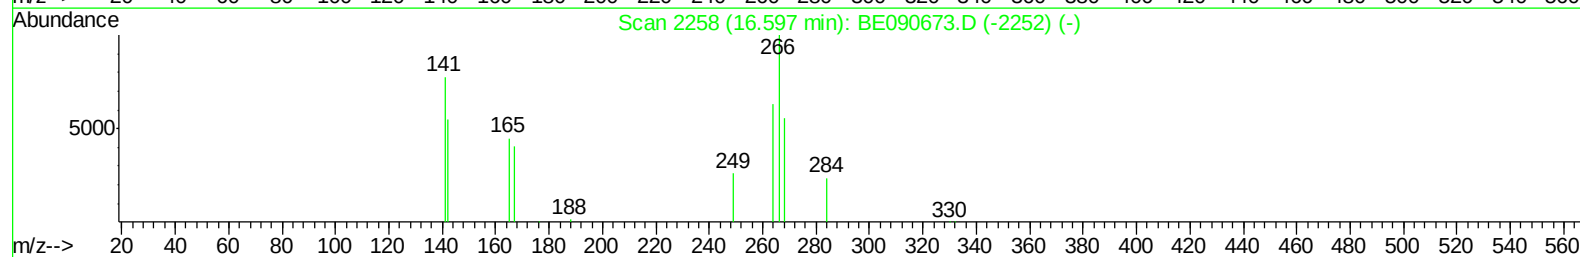
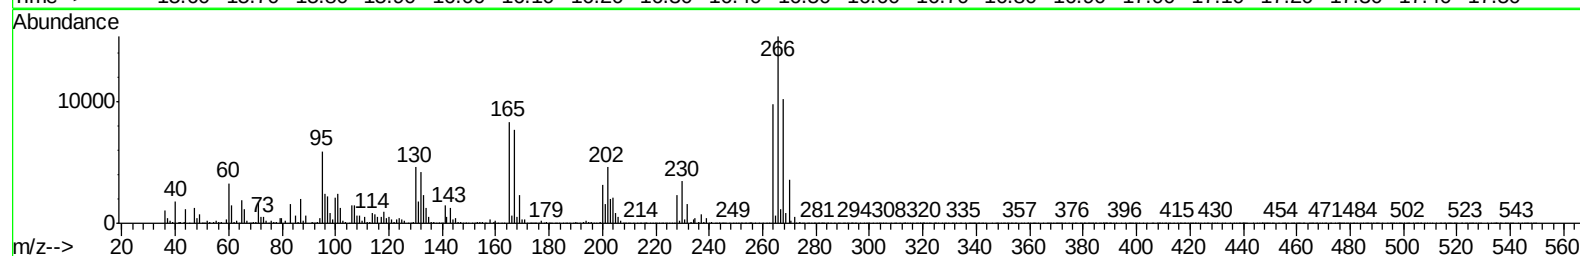


Data Path : Z:\HPCHEM1\BNA E\DATA\BE091715\
Data File : BE090873.D
Acq On : 17 Sep 2015 20:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 01:33:41 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 11:40:50 2015
Response via : Initial Calibration

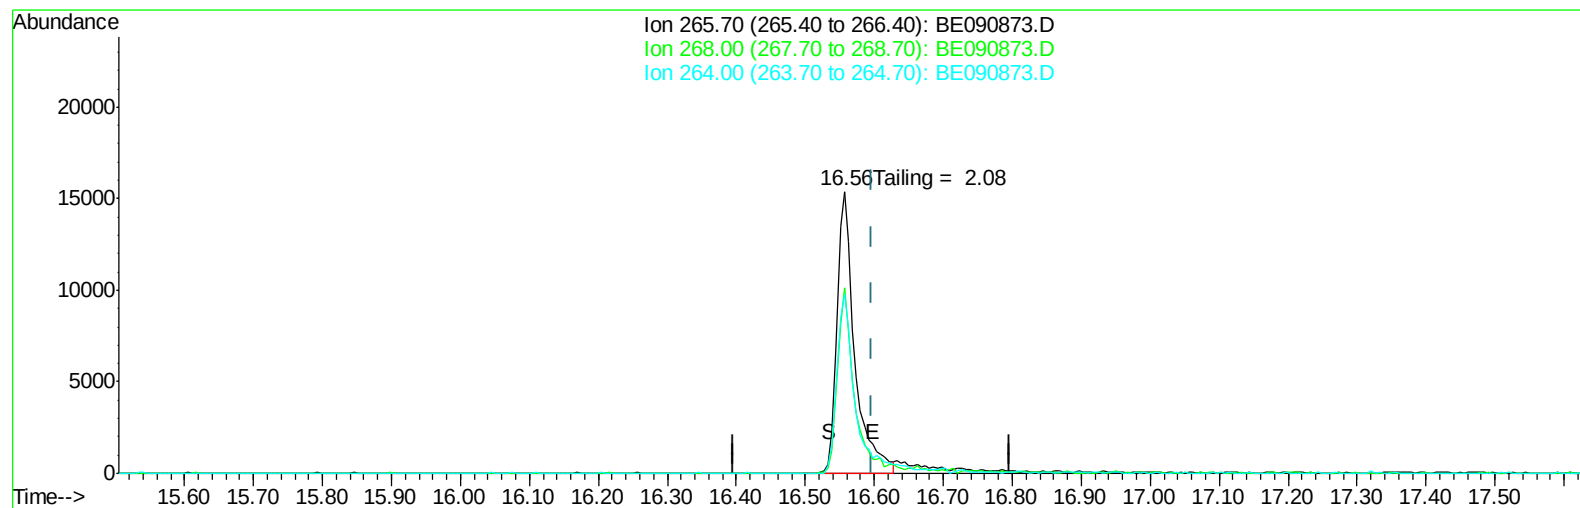

TIC: BE090873.D

(21) Pentachlorophenol

16.556min (-0.041) 116496.19ng

response 27455

Ion	Exp%	Act%
265.70	100	100
268.00	62.00	66.14
264.00	67.40	63.44
0.00	0.00	0.00