

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091715\
 Data File : BE090858.D
 Acq On : 17 Sep 2015 10:26
 Operator : UM/IZ
 Sample : G3677-02
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 091415-D534-F-D-M

Quant Time: Sep 17 11:41:40 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 11:40:50 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	42306	5.00	ng	-0.01
6) Naphthalene-d8	10.30	136	196030	5.00	ng	0.00
12) Acenaphthene-d10	14.16	164	108601	5.00	ng	0.00
18) Phenanthrene-d10	16.91	188	270372	5.00	ng	0.00
25) Chrysene-d12	21.07	240	308778	5.00	ng	0.00
32) Perylene-d12	23.35	264	273893	5.00	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.18	112	33944	4.12	ng	-0.01
5) Phenol-d6	6.74	99	27781	2.36	ng	0.00
7) Nitrobenzene-d5	8.70	82	53897	4.16	ng	0.00
13) 2,4,6-Tribromophenol	15.67	330	30063	9.40	ng	0.00
14) 2-Fluorobiphenyl	12.79	172	119117	3.96	ng	0.00
27) Terphenyl-d14	19.52	244	206886	6.06	ng	-0.02
Target Compounds						
30) Bis(2-ethylhexyl)phthalate	20.99	149	2638	0.21	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091715\
Data File : BE090858.D
Acq On : 17 Sep 2015 10:26
Operator : UM/IZ
Sample : G3677-02
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
091415-D534-F-D-M

Quant Time: Sep 17 11:41:40 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 11:40:50 2015
Response via : Initial Calibration

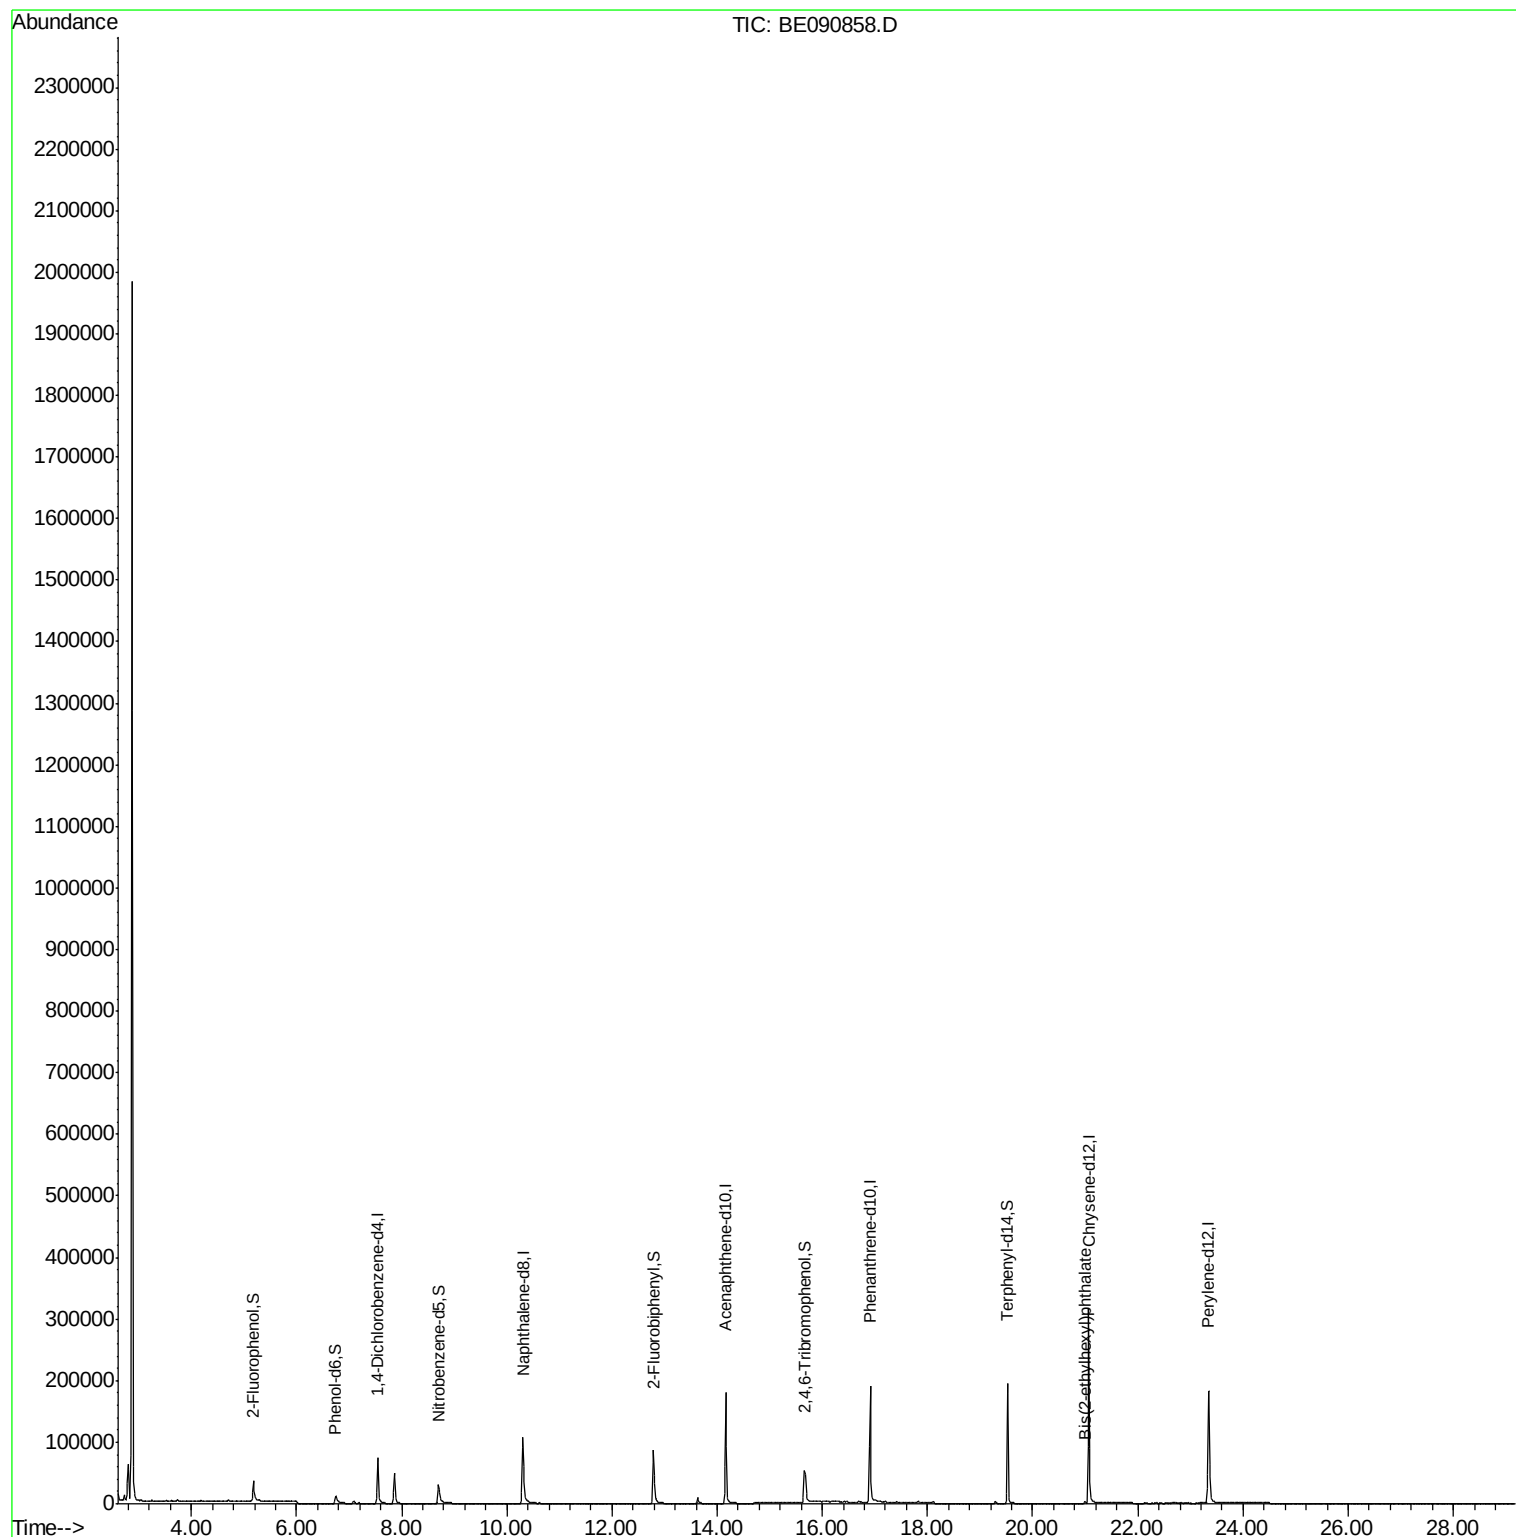

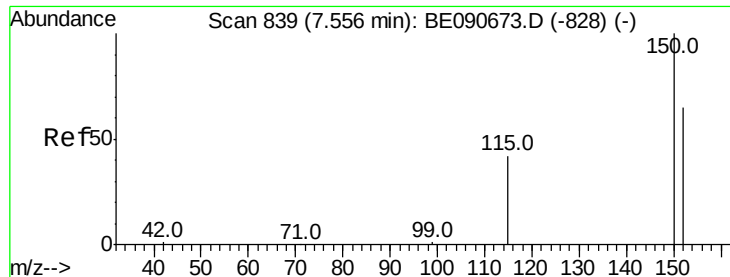

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.54 min Scan# 836

Delta R.T. -0.01 min

Lab File: BE090858.D

Acq: 17 Sep 2015 10:26

Instrument :

BNA_E

ClientSampleId :

091415-D534-F-D-M


Tgt Ion:152 Resp: 42306

Ion Ratio Lower Upper

152 100

150 157.9 122.2 183.4




115 68.4 51.0 76.4

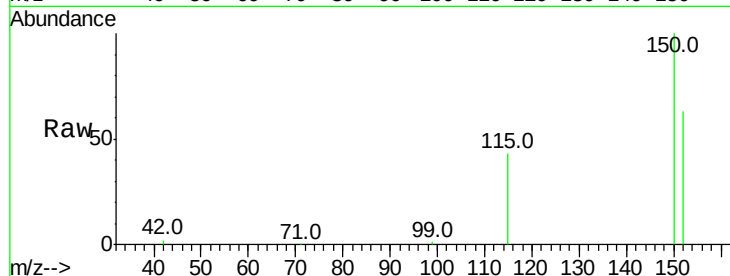

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

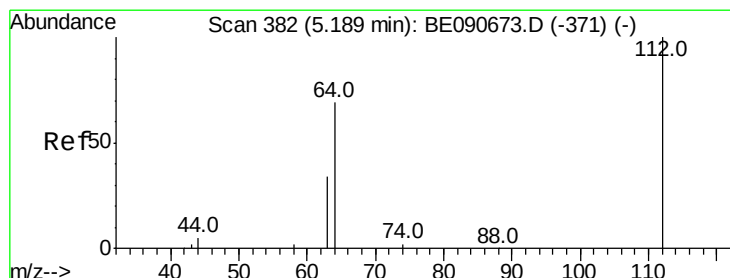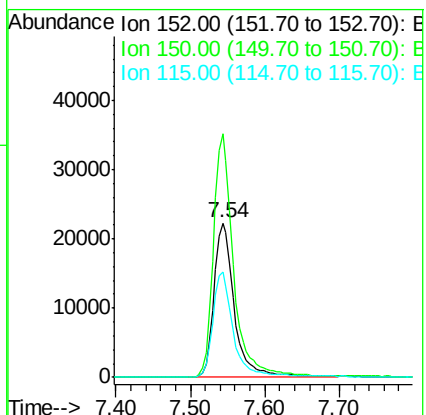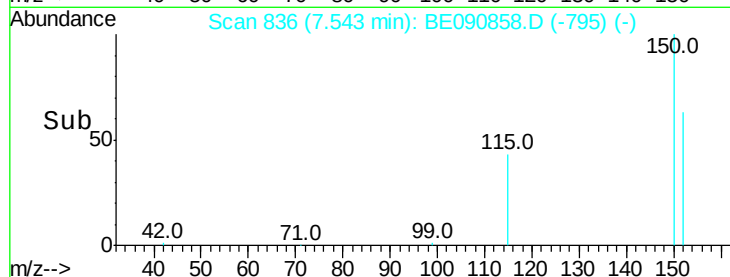

#4

2-Fluorophenol

Concen: 4.12 ng

RT: 5.18 min Scan# 380

Delta R.T. -0.01 min

Lab File: BE090858.D

Acq: 17 Sep 2015 10:26


Tgt Ion:112 Resp: 33944

Ion Ratio Lower Upper

112 100

64 72.4 57.3 85.9



63 37.6 29.2 43.8

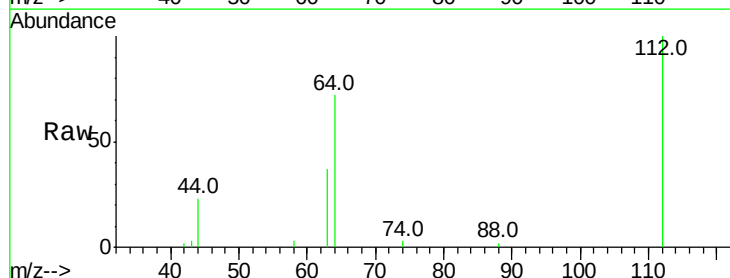


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

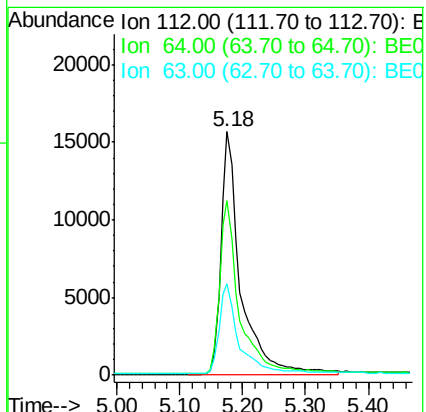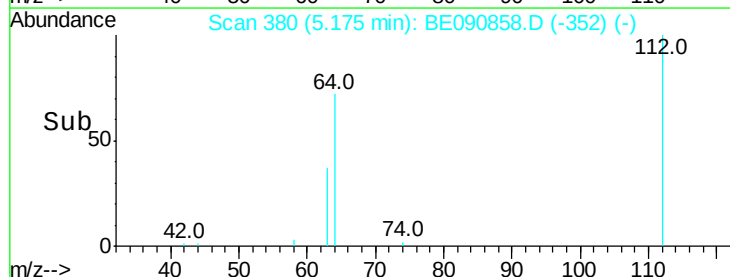



#5

Phenol-d6

Concen: 2.36 ng

RT: 6.74 min Scan# 660

Delta R.T. -0.01 min

Lab File: BE090858.D

Acq: 17 Sep 2015 10:26

Instrument :

BNA_E

ClientSampleId :

091415-D534-F-D-M


Tgt Ion: 99 Resp: 27781

Ion Ratio Lower Upper

99 100

42 21.8 16.8 25.2

71 36.7 28.3 42.5



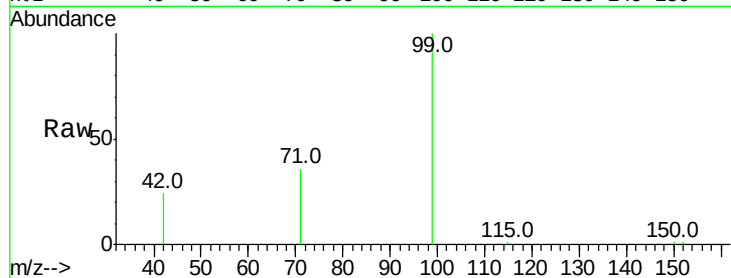


Abundance

Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

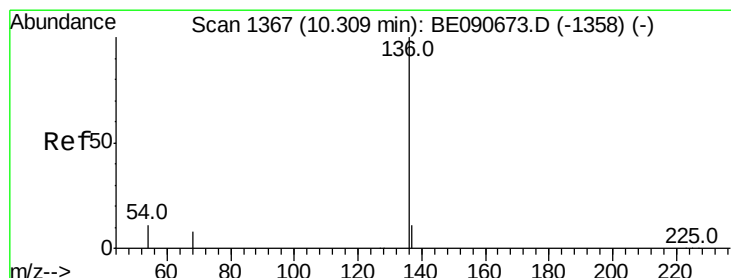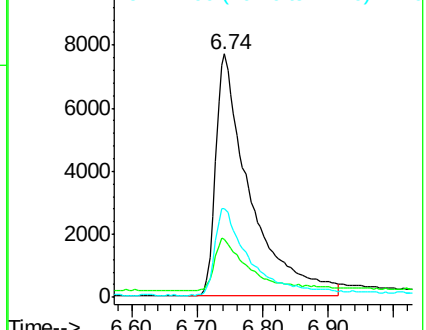

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.30 min Scan# 1366

Delta R.T. -0.01 min

Lab File: BE090858.D

Acq: 17 Sep 2015 10:26

Tgt Ion: 136 Resp: 196030


Ion Ratio Lower Upper

136 100

137 10.9 8.7 13.1

54 11.9 9.0 13.6

68 8.4 6.3 9.5

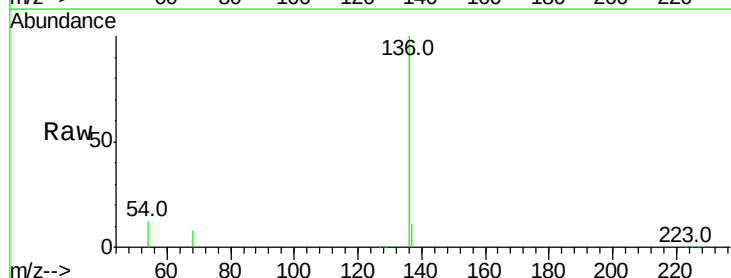



Abundance


Ion 136.00 (135.70 to 136.70): BE0

Ion 137.00 (136.70 to 137.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

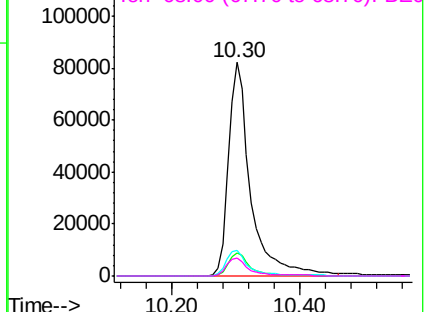

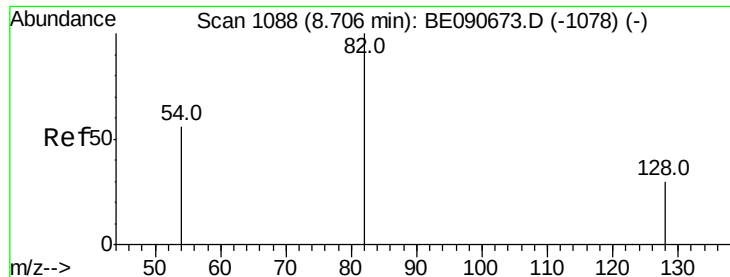

#7

Nitrobenzene-d5

Concen: 4.16 ng

RT: 8.70 min Scan# 1087

Delta R.T. -0.00 min

Lab File: BE090858.D

Acq: 17 Sep 2015 10:26

Instrument :

BNA_E

ClientSampleId :

091415-D534-F-D-M





Tgt Ion: 82 Resp: 53897

Ion Ratio Lower Upper

82 100

128 30.4 25.0 37.4

54 55.8 46.3 69.5

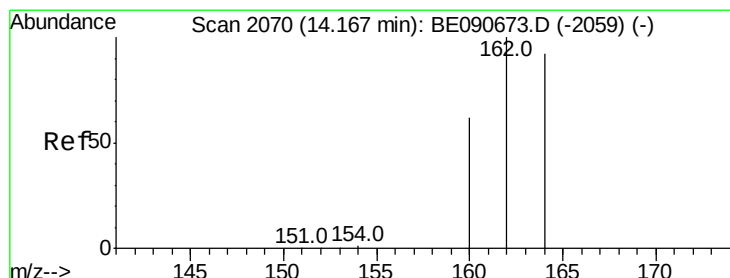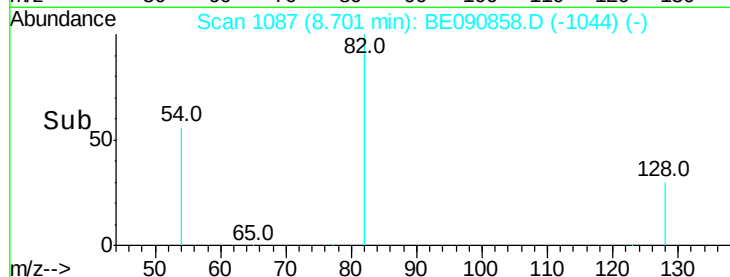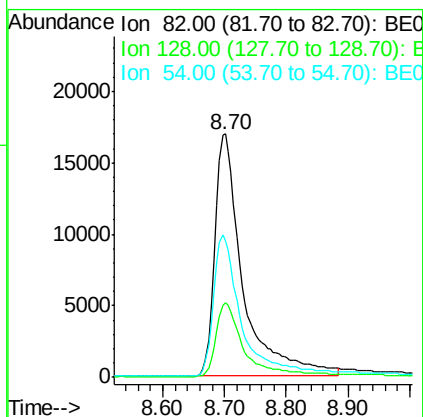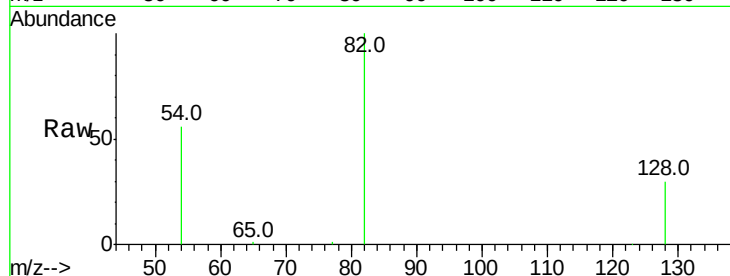

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.16 min Scan# 2069

Delta R.T. -0.01 min

Lab File: BE090858.D

Acq: 17 Sep 2015 10:26




Tgt Ion: 164 Resp: 108601


Ion Ratio Lower Upper

164 100

162 106.7 86.8 130.2

160 56.9 53.9 80.9


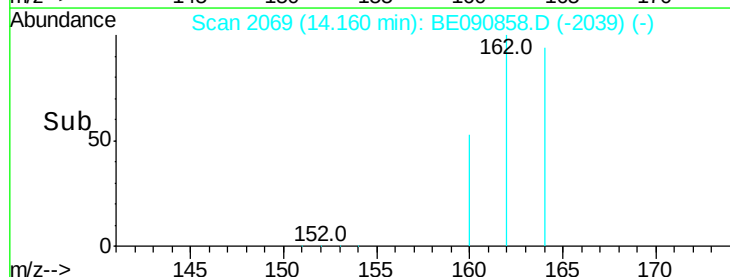
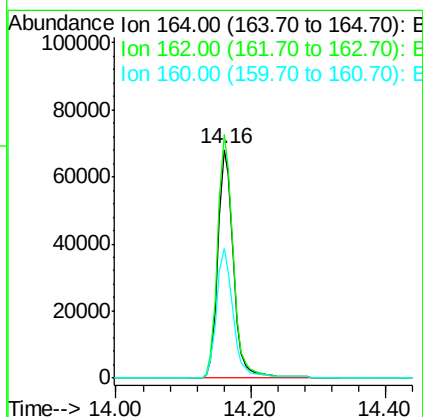
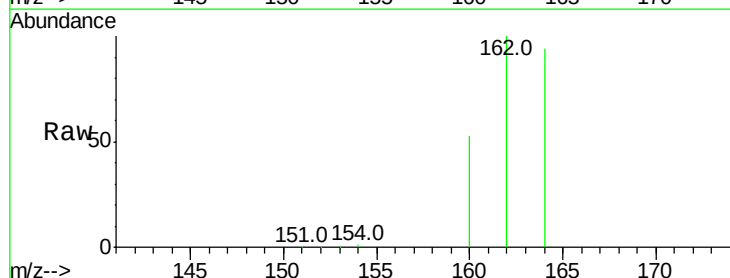




#13
 2,4,6-Tribromophenol
 Concen: 9.40 ng
 RT: 15.67 min Scan# 2204
 Delta R.T. -0.00 min
 Lab File: BE090858.D
 Acq: 17 Sep 2015 10:26




Instrument :
 BNA_E
 ClientSampleId :
 091415-D534-F-D-M


Tgt Ion:330 Resp: 30063
 Ion Ratio Lower Upper
 330 100
 332 96.1 74.9 112.3
 141 178.6 145.2 217.8

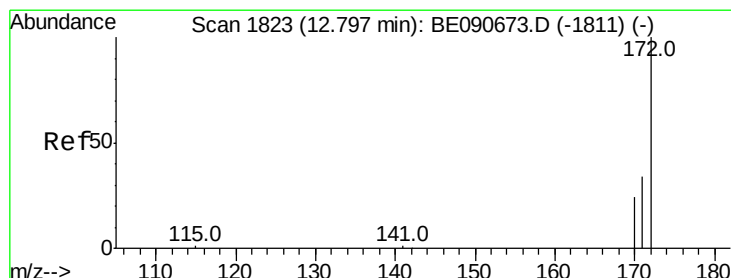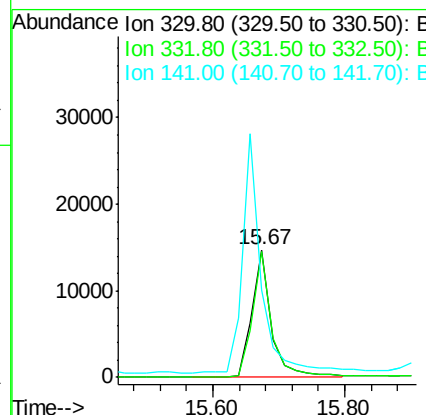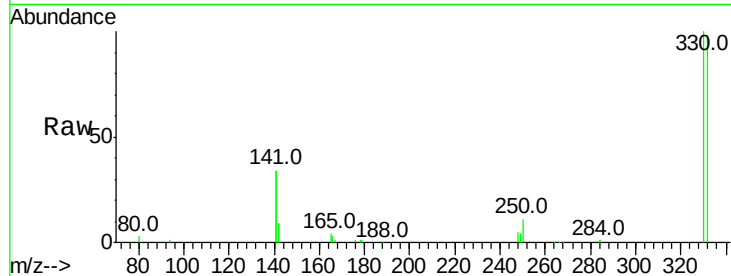

#14
 2-Fluorobiphenyl
 Concen: 3.96 ng
 RT: 12.79 min Scan# 1821
 Delta R.T. -0.01 min
 Lab File: BE090858.D
 Acq: 17 Sep 2015 10:26

Tgt Ion:172 Resp: 119117
 Ion Ratio Lower Upper
 172 100
 171 35.1 27.8 41.8
 170 23.8 19.8 29.6

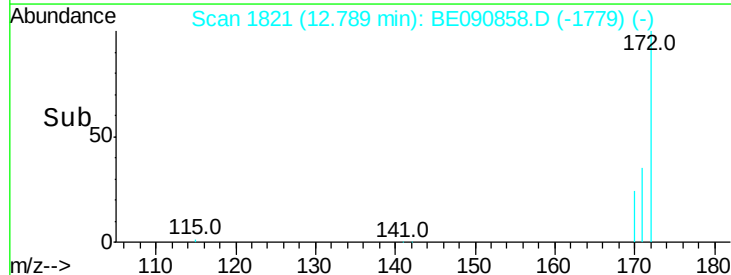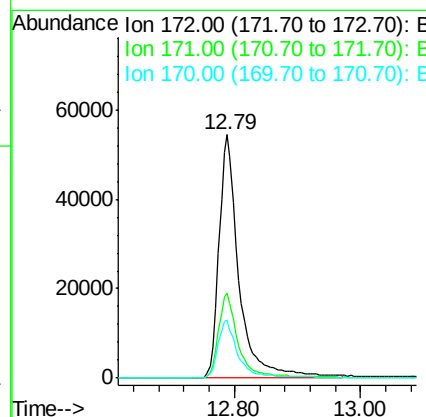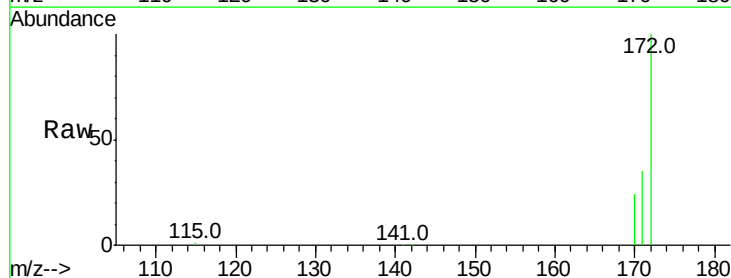



#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.91 min Scan# 2275

Delta R.T. -0.00 min

Lab File: BE090858.D

Acq: 17 Sep 2015 10:26

Instrument :

BNA_E

ClientSampleId :

091415-D534-F-D-M


Tgt Ion:188 Resp: 270372

Ion Ratio Lower Upper

188 100

94 7.9 10.3 15.5#




80 8.4 11.0 16.6#

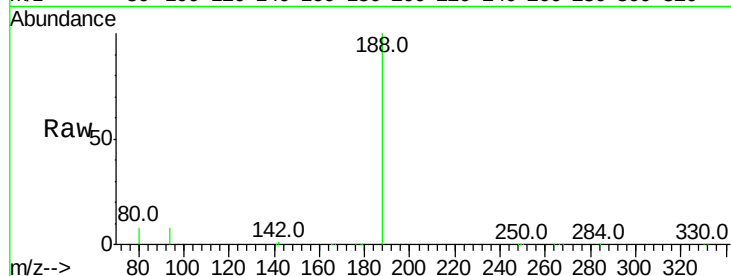

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

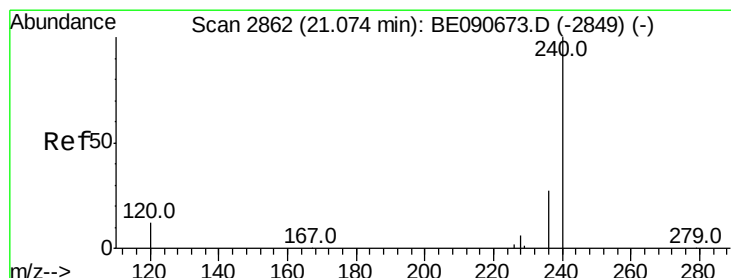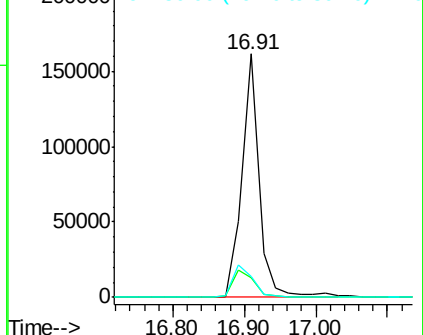

#25

Chrysene-d12

Concen: 5.00 ng

RT: 21.07 min Scan# 2860

Delta R.T. -0.01 min

Lab File: BE090858.D

Acq: 17 Sep 2015 10:26


Tgt Ion:240 Resp: 308778

Ion Ratio Lower Upper

240 100

120 12.6 10.1 15.1



236 27.2 21.9 32.9

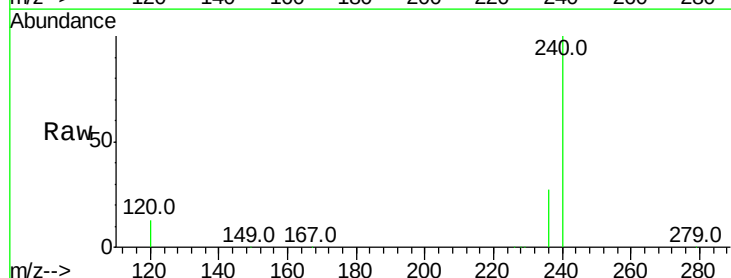


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E




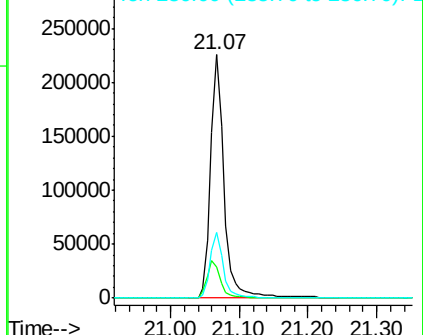


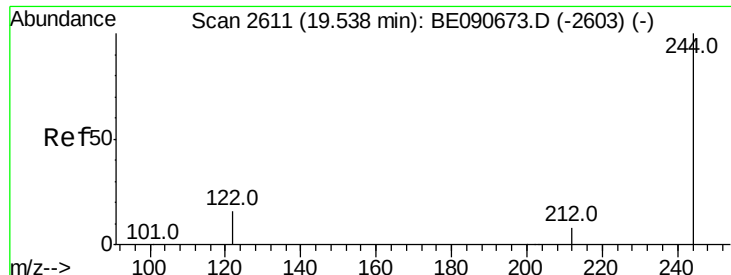

#27
 Terphenyl-d14
 Concen: 6.06 ng
 RT: 19.52 min Scan# 2607
 Delta R.T. -0.02 min
 Lab File: BE090858.D
 Acq: 17 Sep 2015 10:26




Instrument :
 BNA_E
 ClientSampleId :
 091415-D534-F-D-M


Tgt Ion: 244 Resp: 206886
 Ion Ratio Lower Upper
 244 100
 212 8.3 6.9 10.3
 122 16.1 12.9 19.3

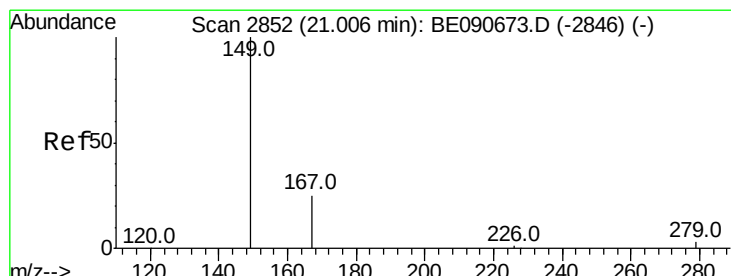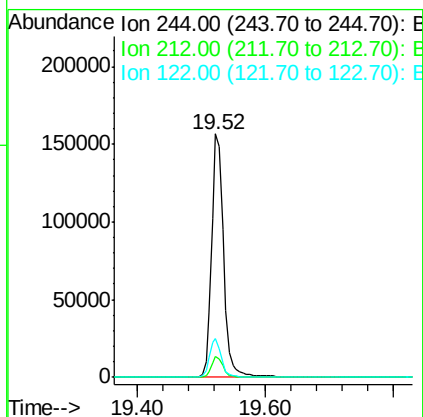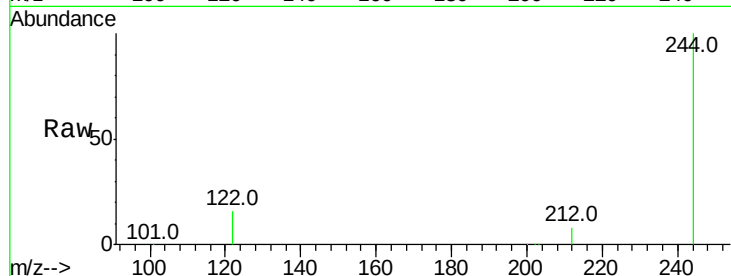

#30
 Bis(2-ethylhexyl)phthalate
 Concen: 0.21 ng
 RT: 20.99 min Scan# 2849
 Delta R.T. -0.01 min
 Lab File: BE090858.D
 Acq: 17 Sep 2015 10:26

Tgt Ion: 149 Resp: 2638
 Ion Ratio Lower Upper
 149 100
 167 25.0 20.1 30.1
 279 3.2 2.3 3.5

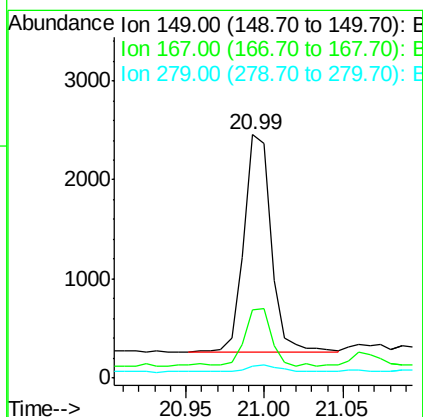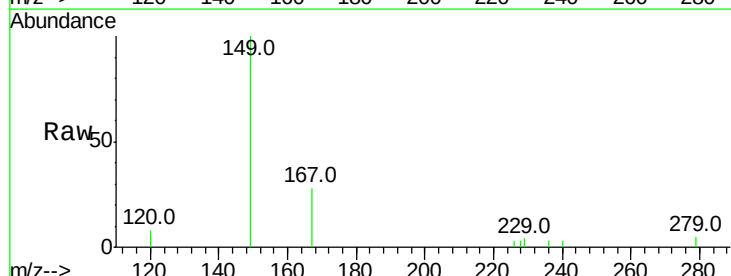

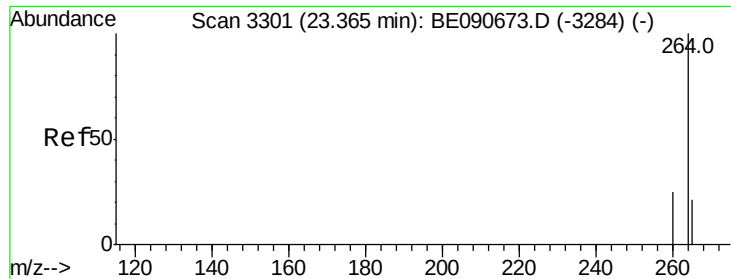

#32
Perylene-d12
Concen: 5.00 ng
RT: 23.35 min Scan# 3296
Delta R.T. -0.02 min
Lab File: BE090858.D
Acq: 17 Sep 2015 10:26

Instrument :
BNA_E
ClientSampleId :
091415-D534-F-D-M

Tgt Ion: 264 Resp: 273893
Ion Ratio Lower Upper
264 100
260 25.2 19.7 29.5
265 21.6 17.5 26.3

