


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091715\
 Data File : BE090856.D
 Acq On : 17 Sep 2015 9:02
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 02 11:40:50 2015

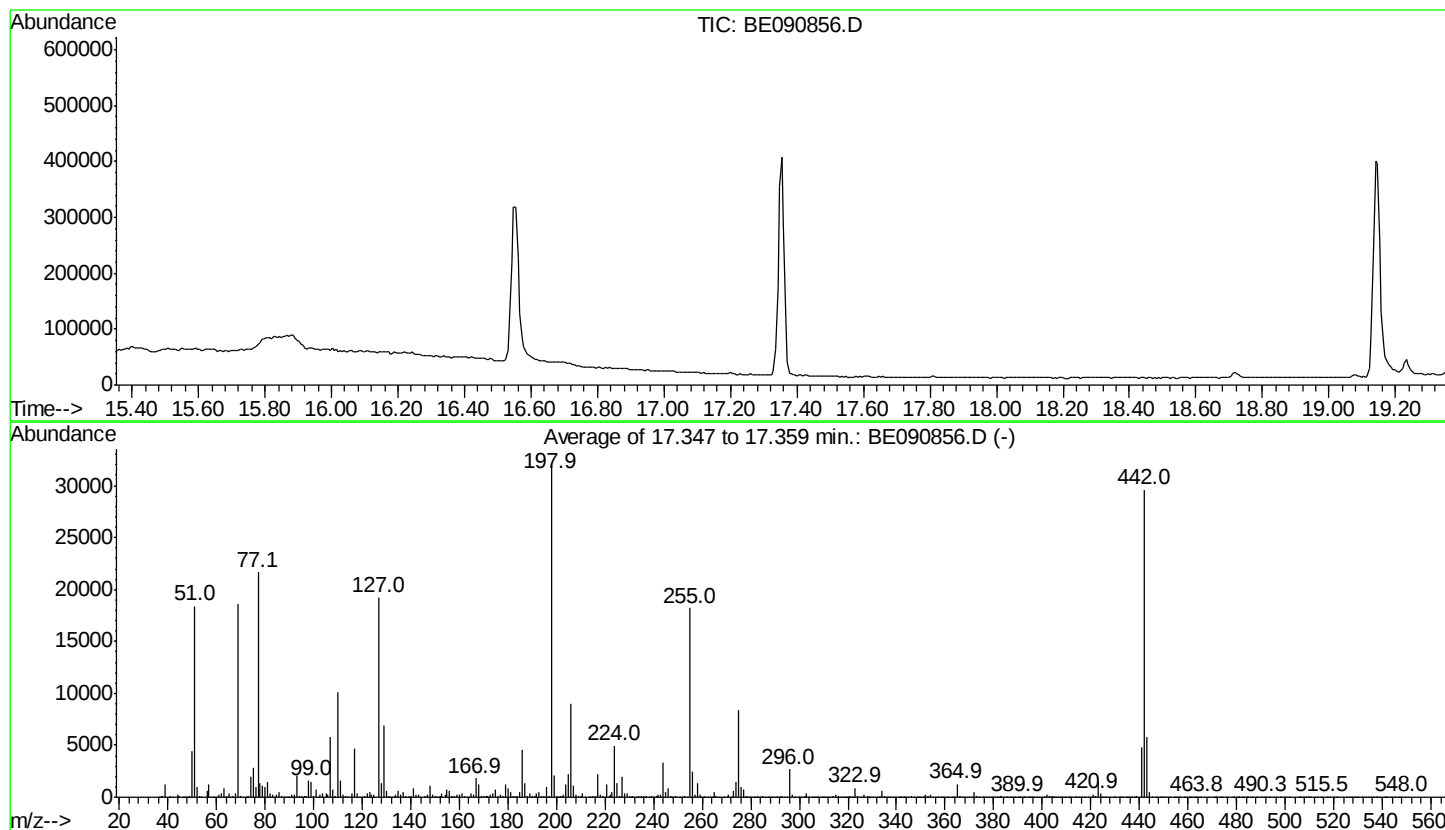

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.6	18373	PASS
68	69	0.00	2	2.0	378	PASS
69	198	0.00	100	58.2	18578	PASS
70	69	0.00	2	0.4	74	PASS
127	198	10	80	60.1	19186	PASS
197	198	0.00	2	0.6	180	PASS
198	198	100	100	100.0	31925	PASS
199	198	5	9	6.7	2126	PASS
275	198	10	60	26.1	8333	PASS
365	198	1	100	3.9	1253	PASS
441	442	0.01	24	16.2	4788	PASS
442	198	50	100	92.8	29635	PASS
443	442	15	24	19.7	5851	PASS