


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091715\
 Data File : BE090873.D
 Acq On : 17 Sep 2015 20:17
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 02 11:40:50 2015

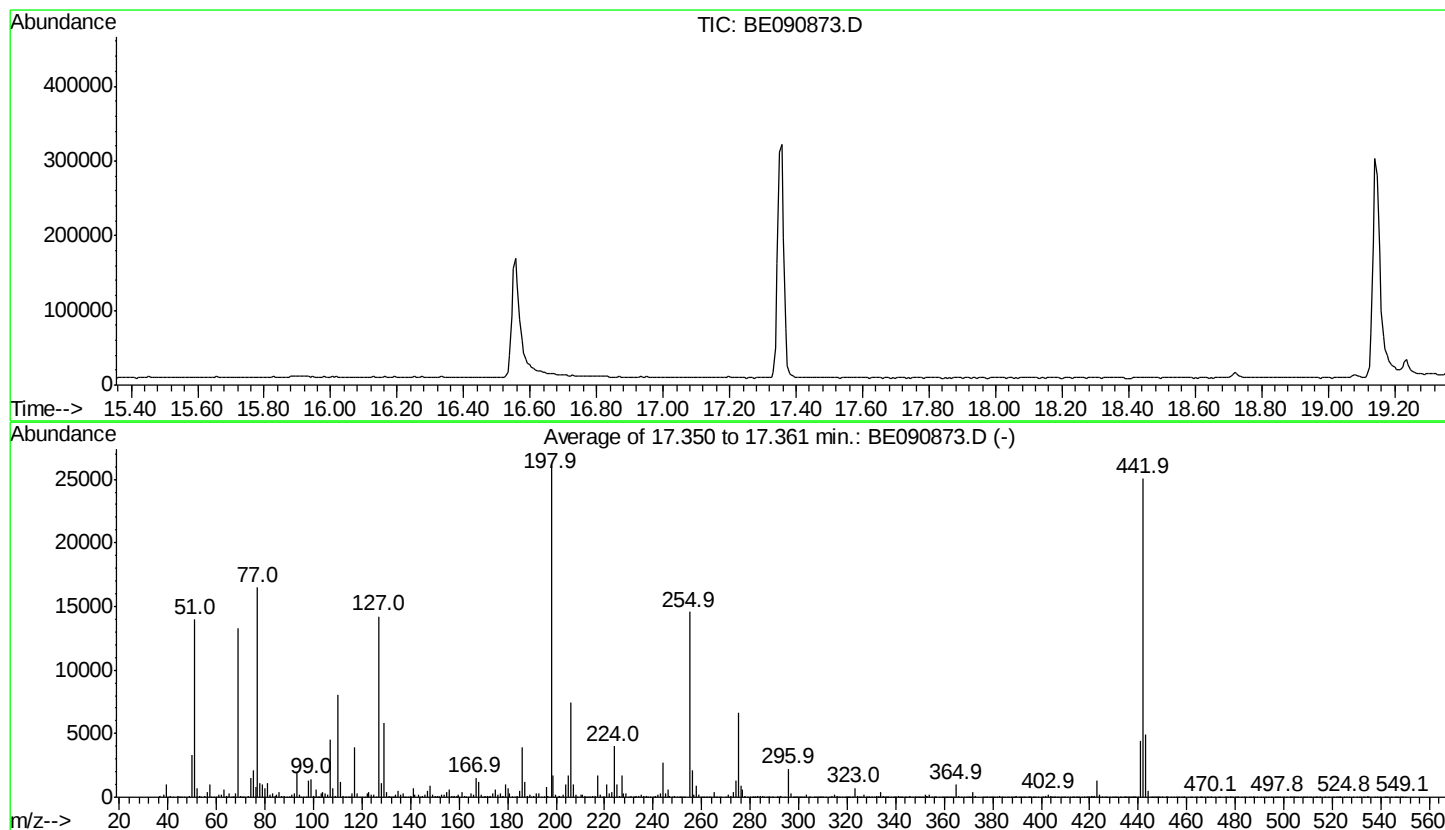

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	13958	PASS
68	69	0.00	2	2.3	307	FAIL*
69	198	0.00	100	50.9	13264	PASS
70	69	0.00	2	0.6	79	PASS
127	198	10	80	54.5	14215	PASS
197	198	0.00	2	0.3	71	PASS
198	198	100	100	100.0	26066	PASS
199	198	5	9	6.7	1738	PASS
275	198	10	60	25.5	6650	PASS
365	198	1	100	3.8	992	PASS
441	442	0.01	24	17.7	4426	PASS
442	198	50	100	96.0	25033	PASS
443	442	15	24	19.5	4893	PASS