
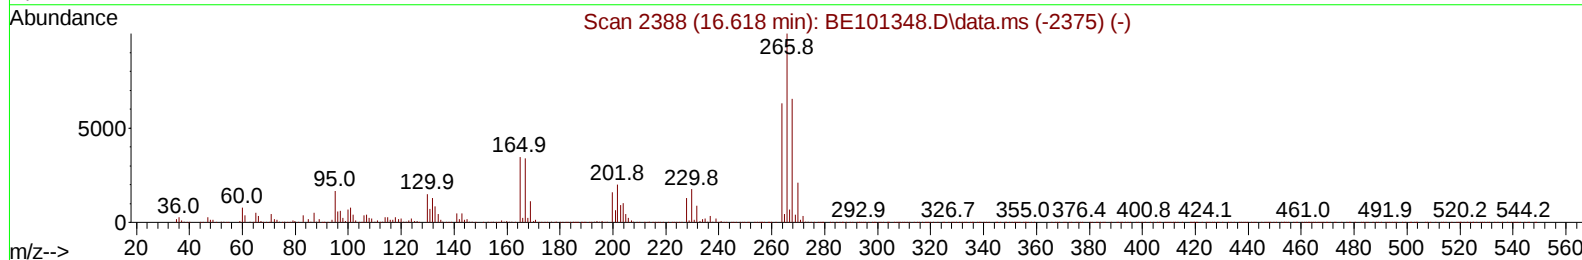
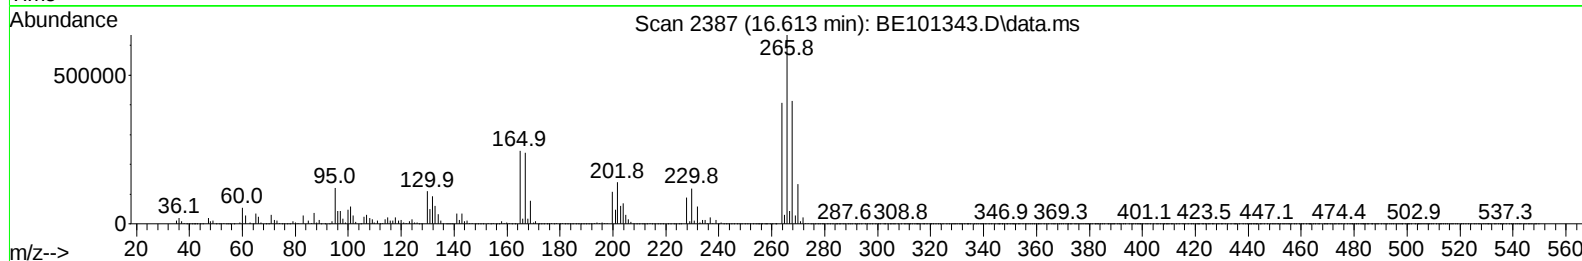


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091724\
Data File : BE101343.D
Acq On : 17 Sep 2024 8:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 04:01:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 17 16:03:42 2024
Response via : Initial Calibration

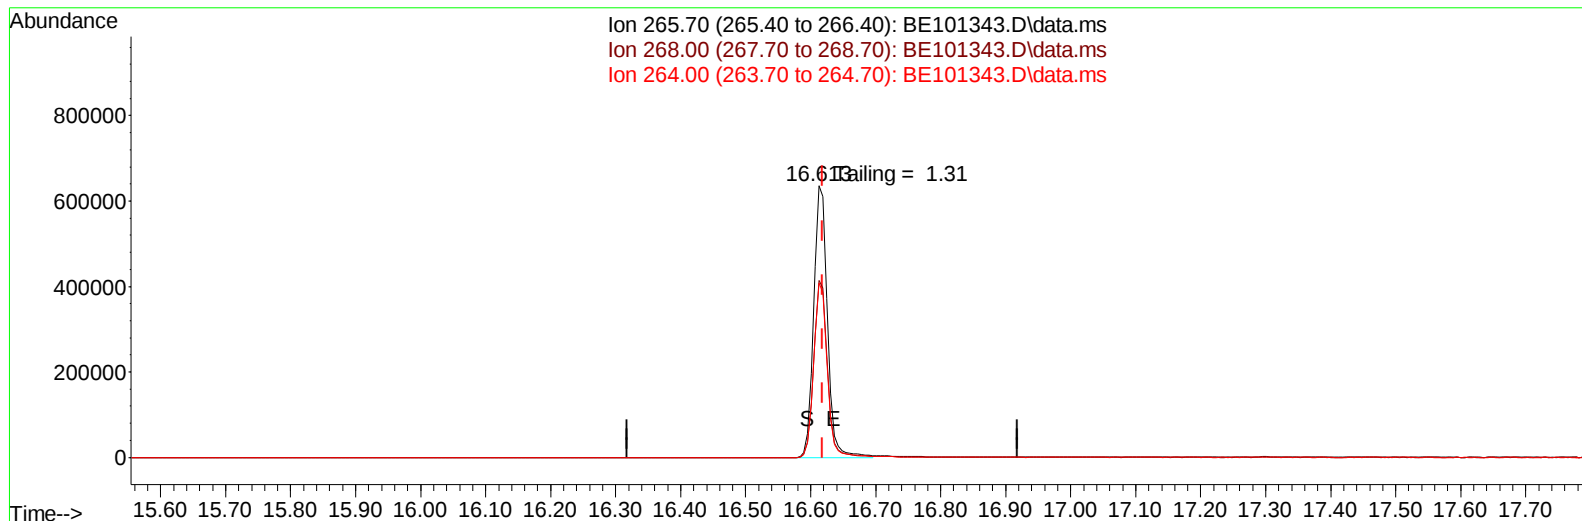




TIC: BE101343.D\data.ms

(70) Pentachlorophenol (C)**16.613min (-0.005) 2670666.80 ng****response 942643**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.23
264.00	63.10	64.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091724\
Data File : BE101343.D
Acq On : 17 Sep 2024 8:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 04:01:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 17 16:03:42 2024
Response via : Initial Calibration

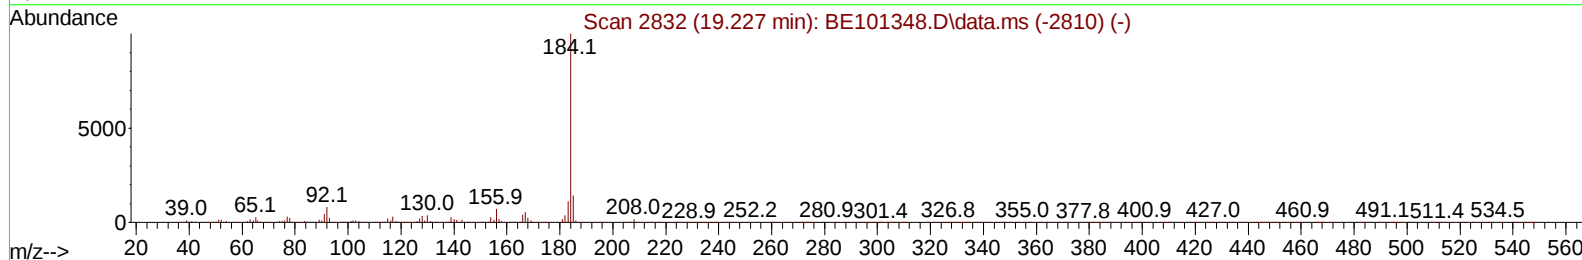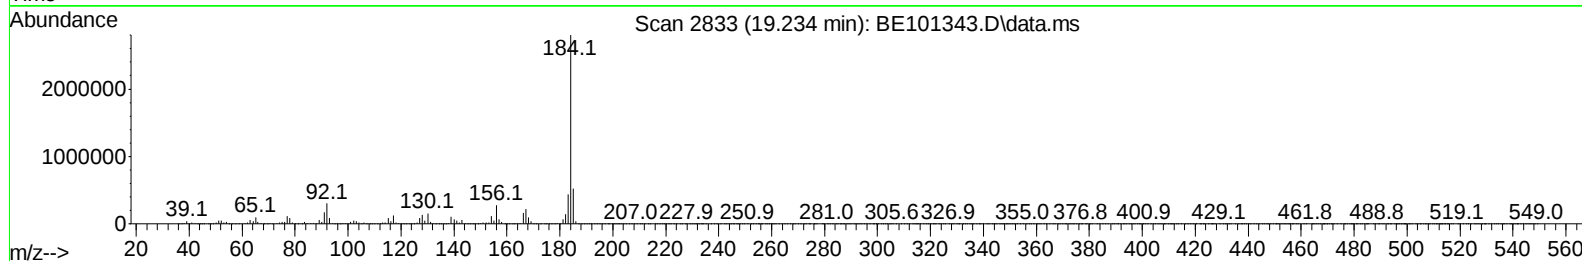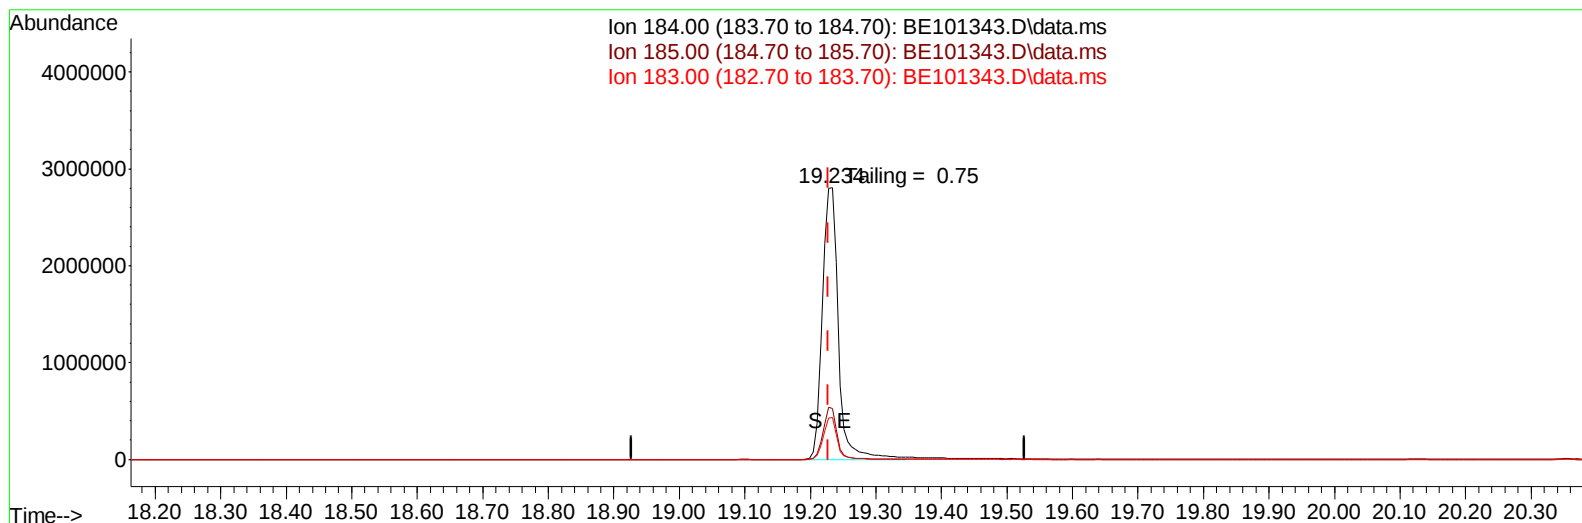

TIC: BE101343.D\data.ms

(77) Benzidine**19.234min (+ 0.007) 3547764.05 ng****response 4828237**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	18.76#
183.00	11.40	15.54#
0.00	0.00	0.00