
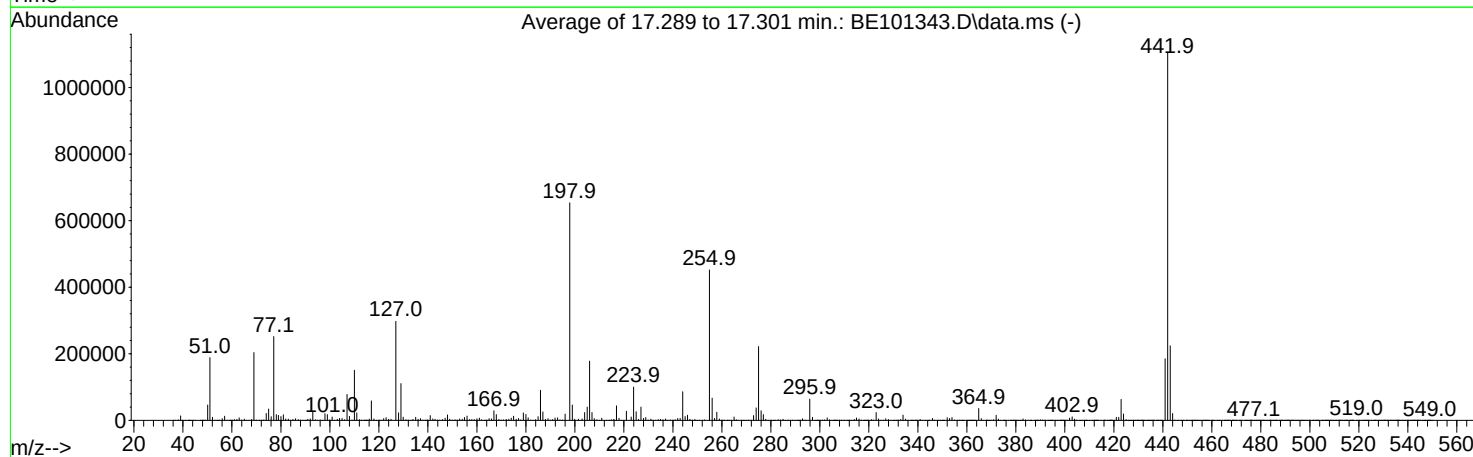


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091724\
Data File : BE101343.D
Acq On : 17 Sep 2024 8:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 17 16:03:42 2024

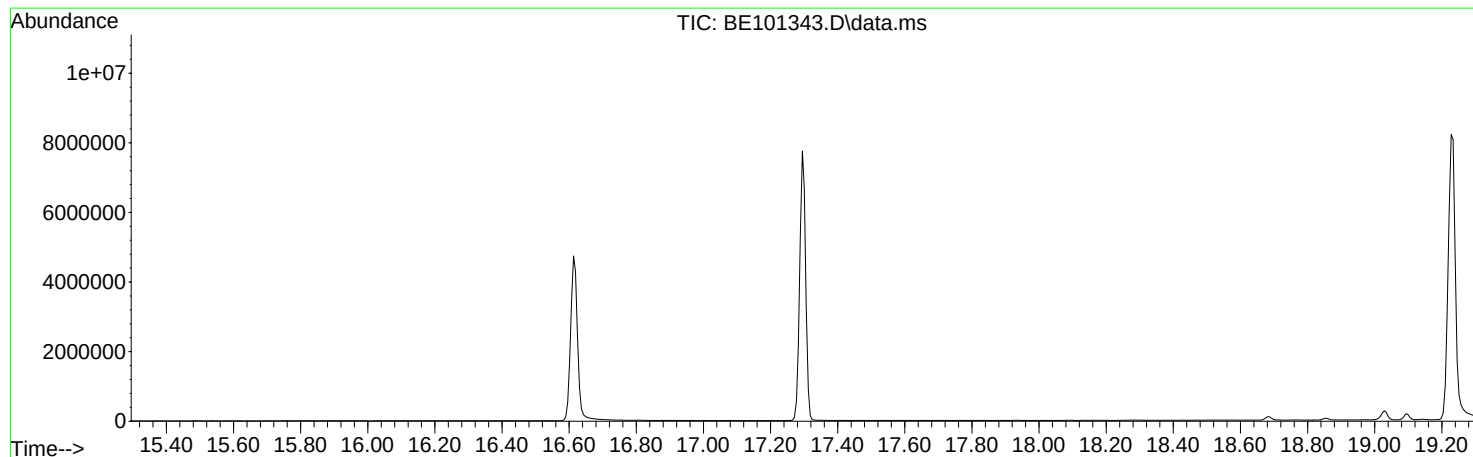




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	188579	PASS
68	69	0.00	2	1.5	3133	PASS
69	198	0.00	100	31.2	203775	PASS
70	69	0.00	2	0.6	1169	PASS
127	198	10	80	45.5	297793	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	653863	PASS
199	198	5	9	7.1	46163	PASS
275	198	10	60	33.9	221865	PASS
365	198	1	100	5.4	35523	PASS
441	198	0.01	100	28.3	185290	PASS
442	442	50	100	100.0	1105335	PASS
443	442	15	24	20.3	224043	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091724\
Data File : BE101343.D
Acq On : 17 Sep 2024 8:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Sep 18 04:01:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 17 16:03:42 2024
Response via : Initial Calibration

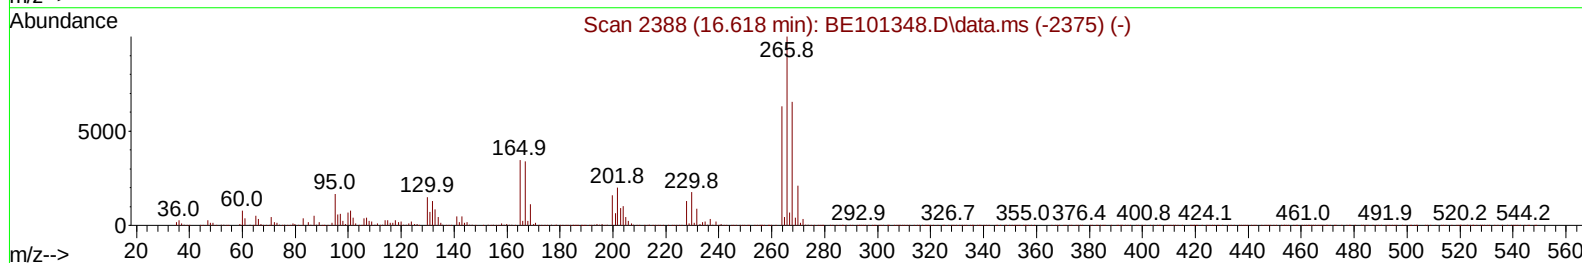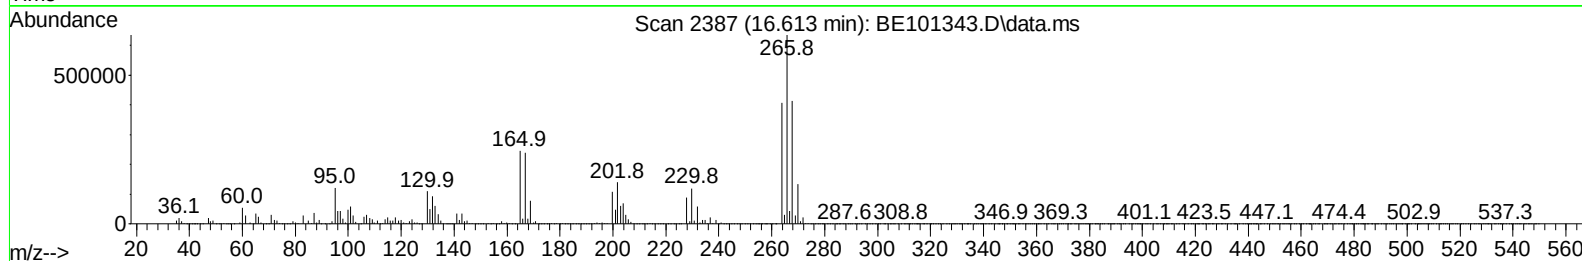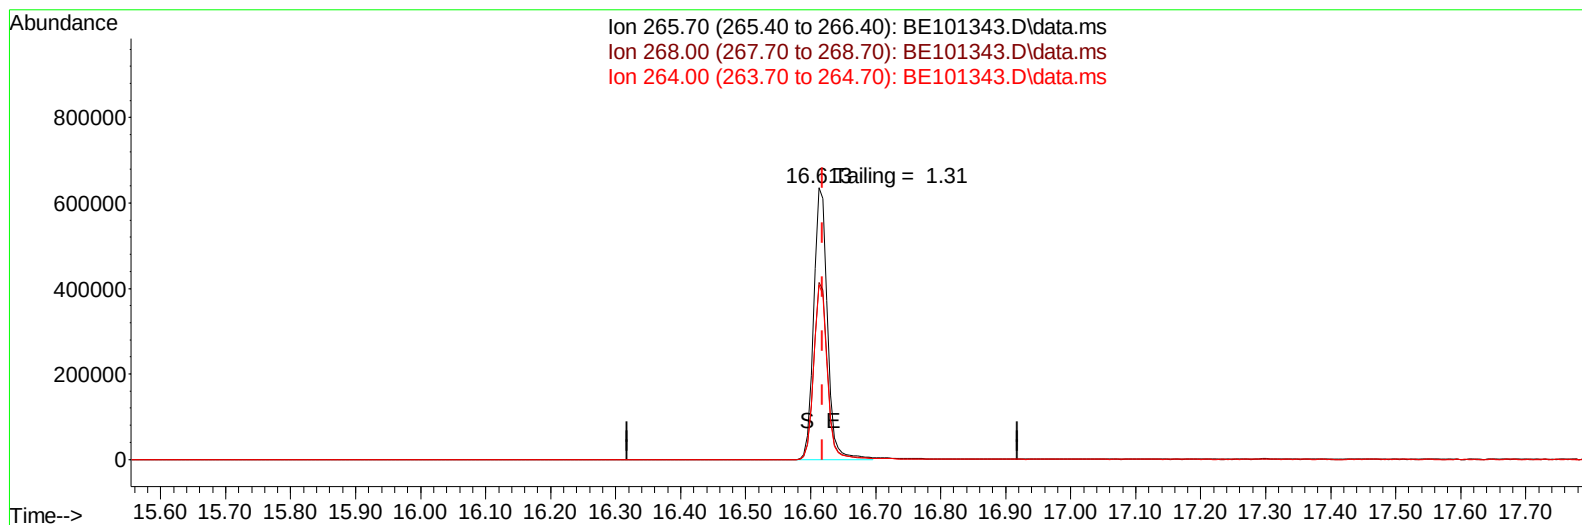

TIC: BE101343.D\data.ms

(70) Pentachlorophenol (C)

16.613min (-0.005) 2670666.80 ng




response 942643

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.23
264.00	63.10	64.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091724\
Data File : BE101343.D
Acq On : 17 Sep 2024 8:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Sep 18 04:01:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 17 16:03:42 2024
Response via : Initial Calibration

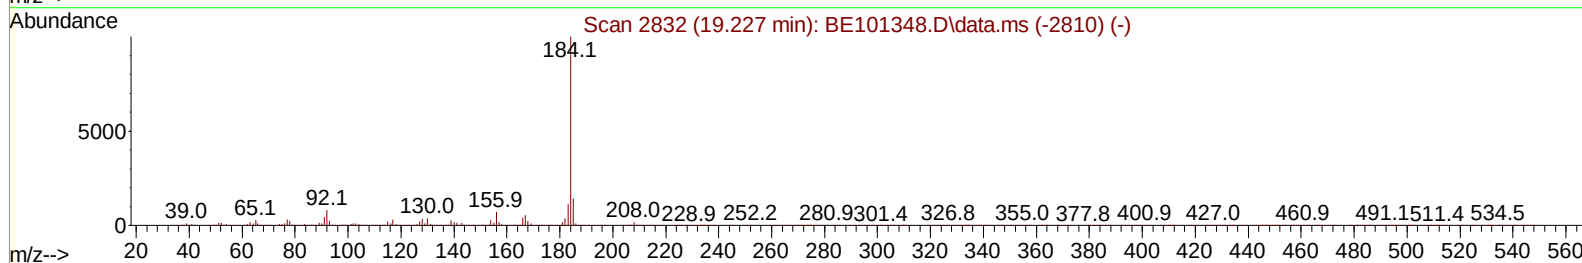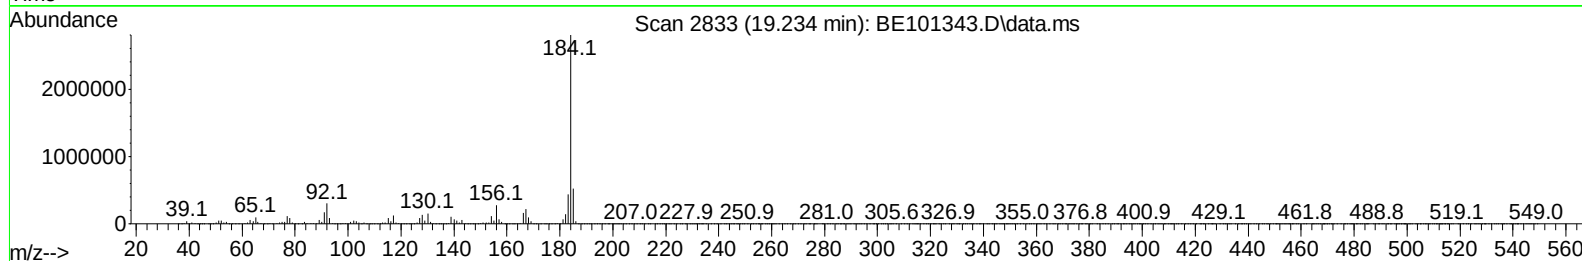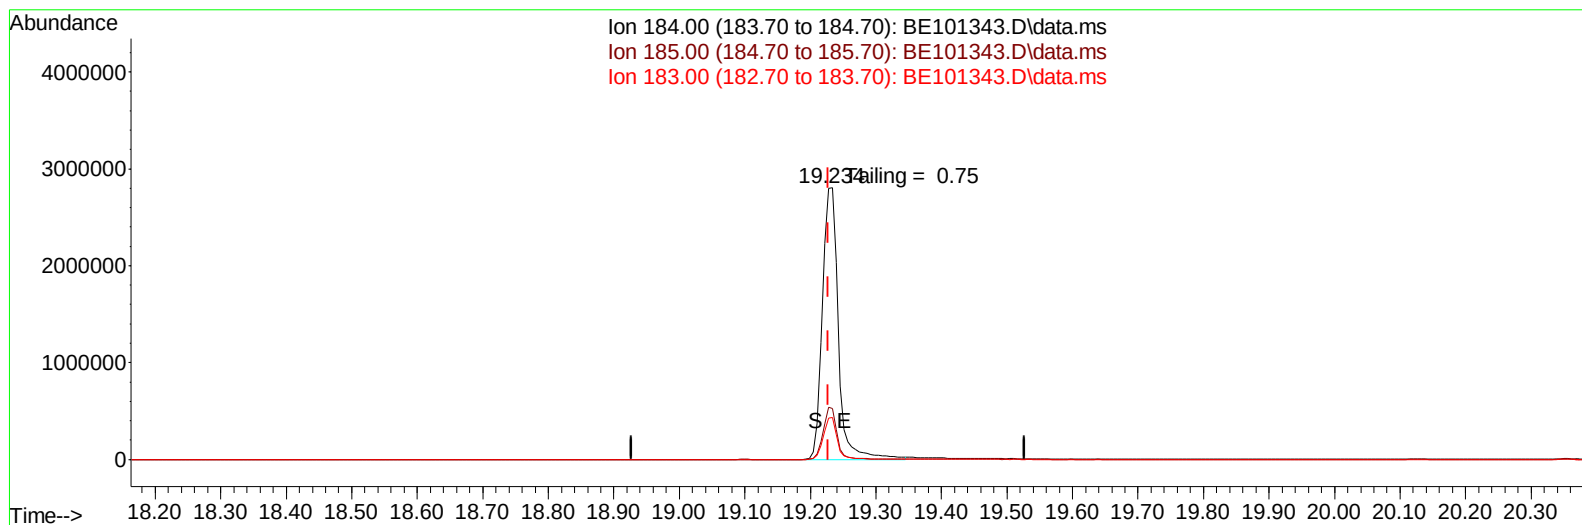

TIC: BE101343.D\data.ms

(77) Benzidine

19.234min (+ 0.007) 3547764.05 ng

response 4828237

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	18.76#
183.00	11.40	15.54#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/17/2024	BNA_E	<u>BE101343.D</u>
Compound Name	Response	Retention Time
DDT	2597503	20.356
DDD	42323	19.921
DDE	1380	19.41
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43703	2641206	1.65

Instrument :
BNA_E
ClientSampleId :
DFTPP