
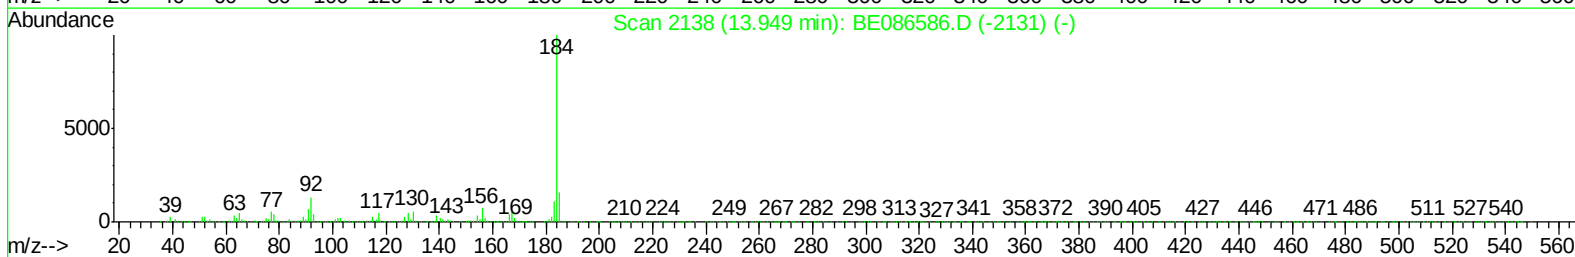
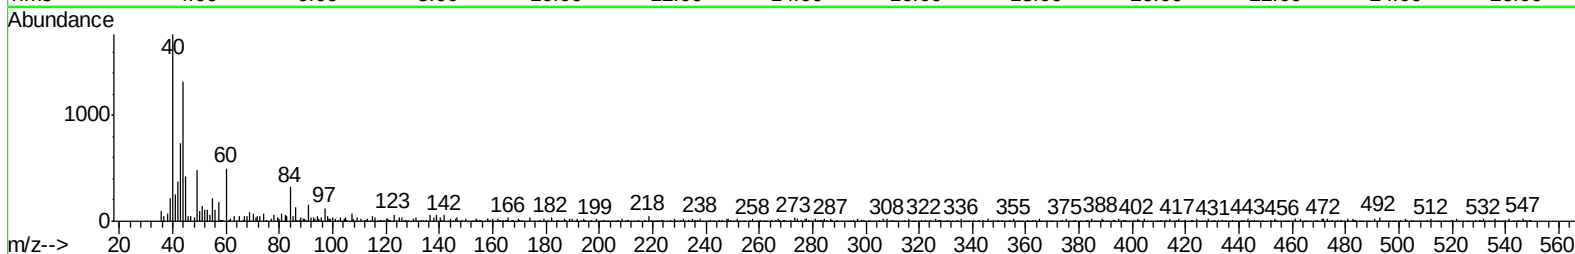


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091815\
 Data File : BE090881.D
 Acq On : 18 Sep 2015 9:33
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 18:39:22 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-BE070214.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 02 16:35:20 2014
 Response via : Initial Calibration

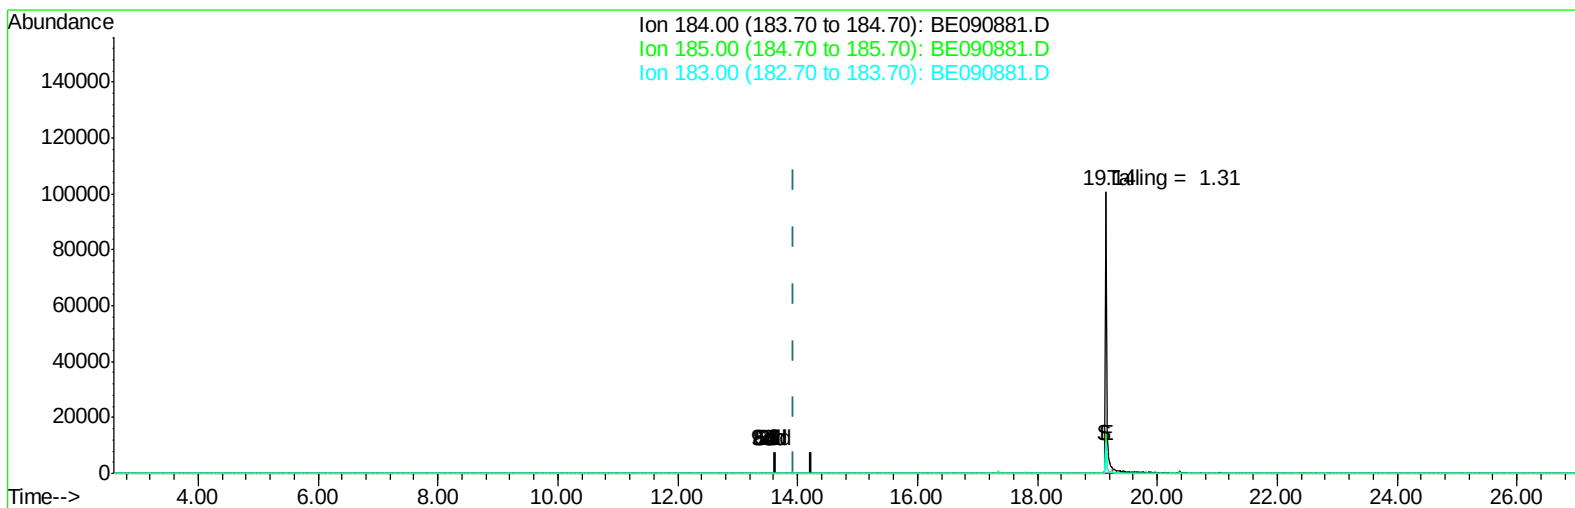

TIC: BE090881.D

(76) Benzidine




13.581min (-0.367) 29.36ng

response 28

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	6.67#
183.00	11.20	6.67#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091815\
Data File : BE090881.D
Acq On : 18 Sep 2015 9:33
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 18:39:22 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-BE070214.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 02 16:35:20 2014
Response via : Initial Calibration

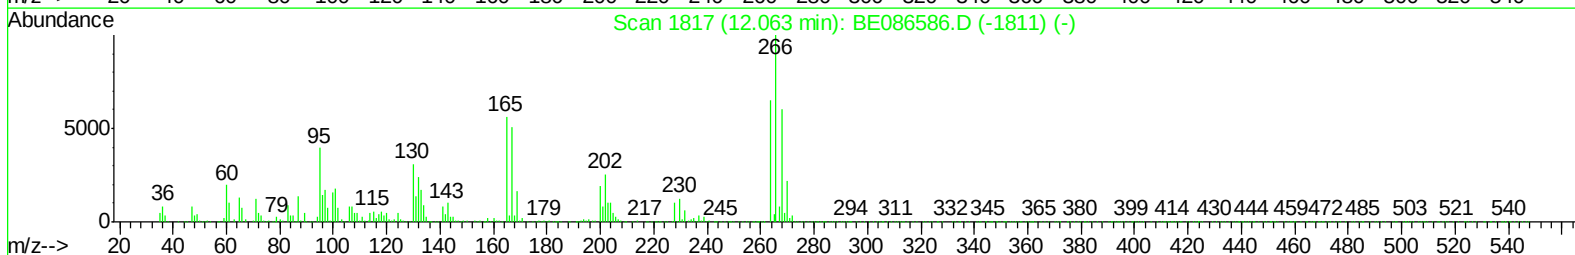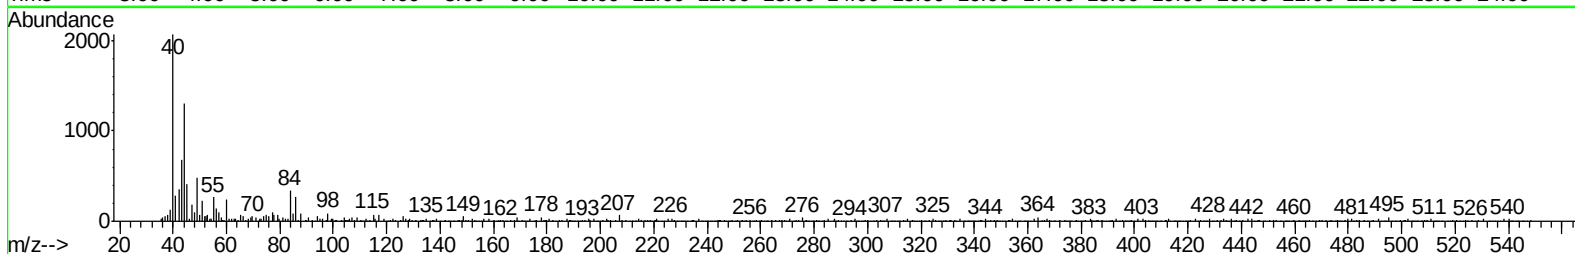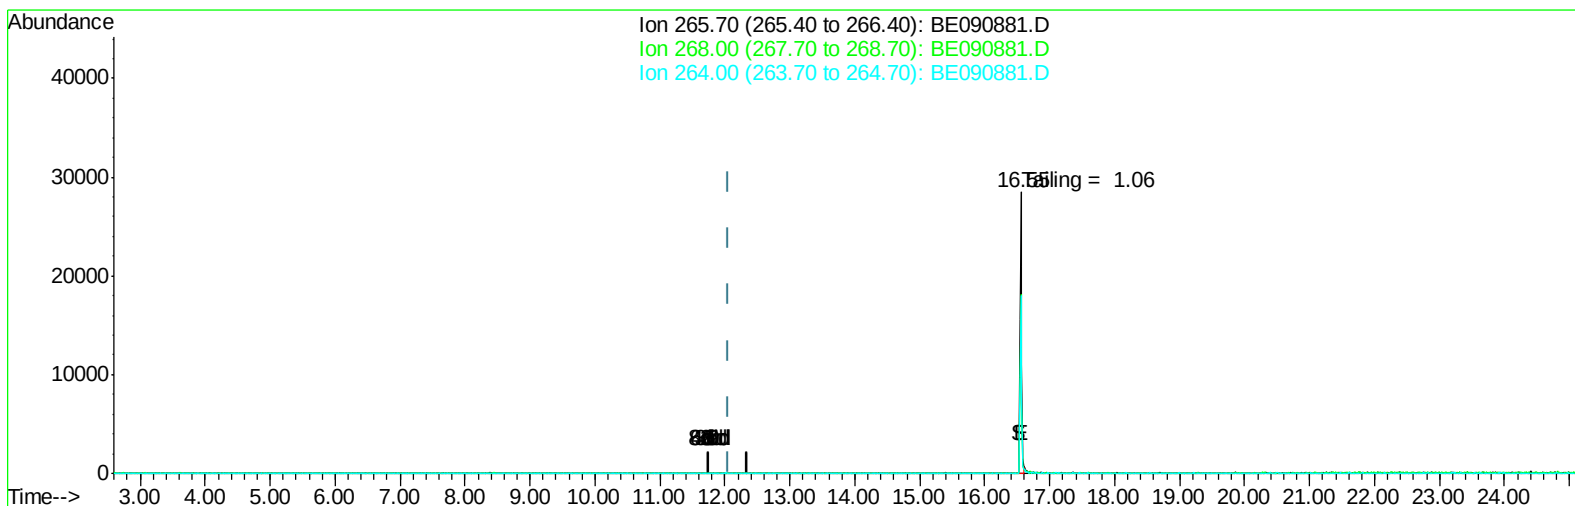

TIC: BE090881.D

(69) Pentachlorophenol (C)

11.753min (-0.309) 426.03ng

response 21

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	45.00#
264.00	63.00	60.00
0.00	0.00	0.00