
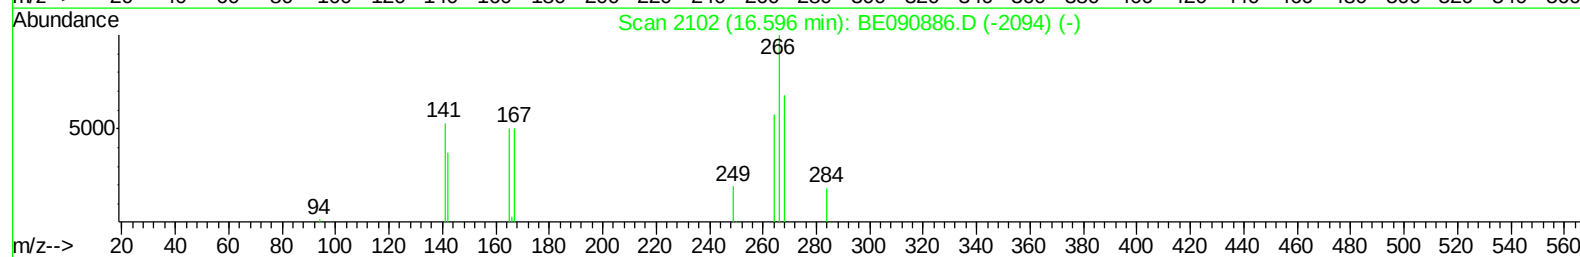
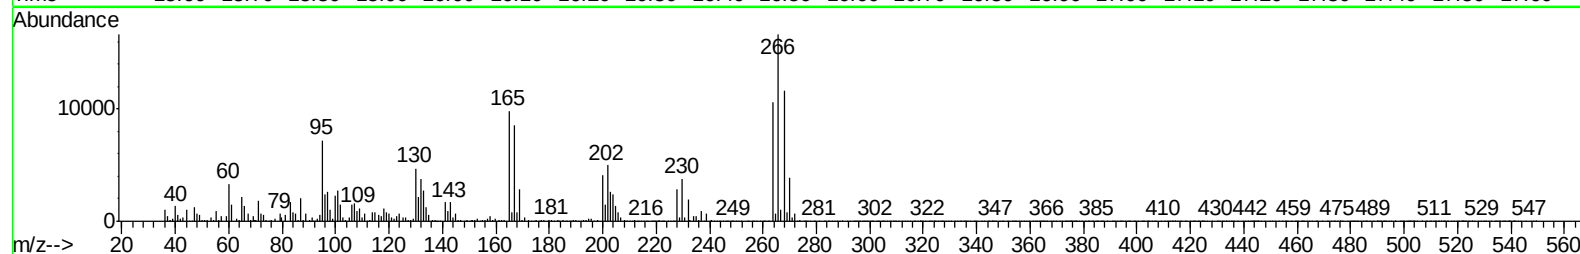


Data Path : Z:\HPCHEM1\BNA E\DATA\BE091815\
Data File : BE090891.D
Acq On : 18 Sep 2015 23:26
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 02:32:45 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE091815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 18 18:17:34 2015
Response via : Initial Calibration

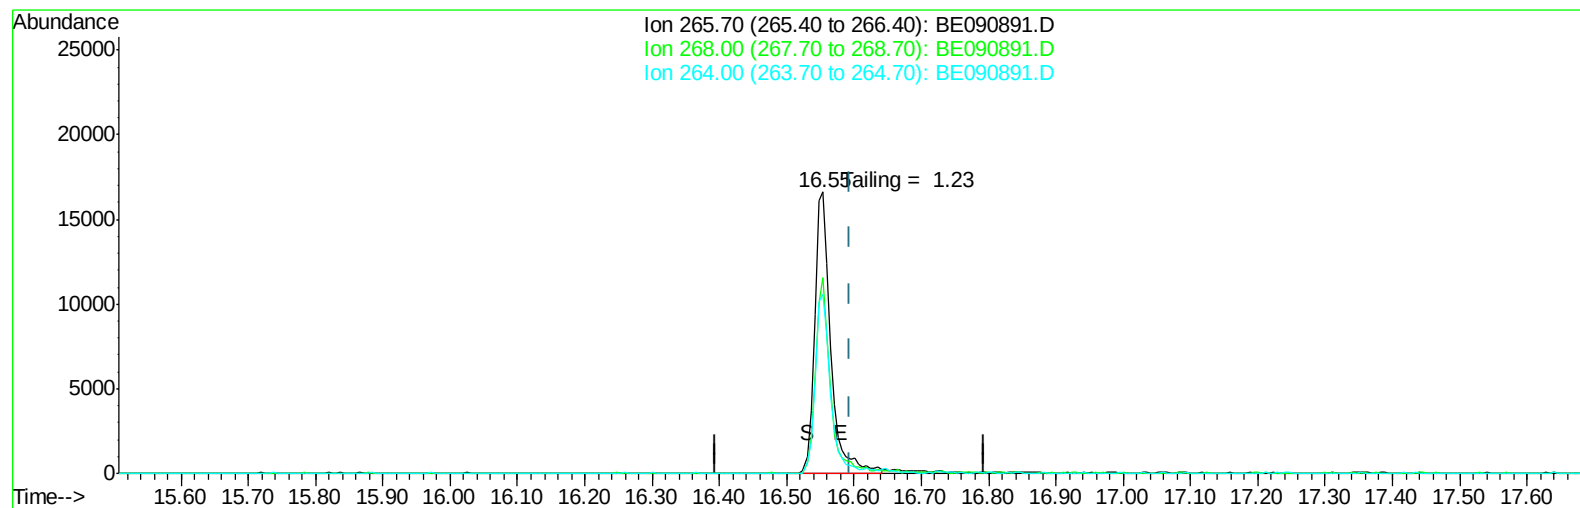

TIC: BE090891.D

(22) Pentachlorophenol

16.553min (-0.042) 4993.41ng

response 28428

Ion	Exp%	Act%
265.70	100	100
268.00	62.00	69.56
264.00	67.40	63.46
0.00	0.00	0.00