

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091815\
 Data File : BE090905.D
 Acq On : 19 Sep 2015 10:31
 Operator : UM/IZ
 Sample : G3723-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 091615-D534-F-U-S

Quant Time: Sep 21 02:45:35 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 18 18:17:34 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	27272	5.00	ng	0.00
7) Naphthalene-d8	10.31	136	116673	5.00	ng	0.00
13) Acenaphthene-d10	14.16	164	63993	5.00	ng	0.00
19) Phenanthrene-d10	16.91	188	154143	5.00	ng	0.00
26) Chrysene-d12	21.07	240	206505	5.00	ng	0.00
33) Perylene-d12	23.35	264	199466	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.18	112	24923	4.06	ng	0.00
5) Phenol-d6	6.75	99	18325	2.16	ng	0.00
8) Nitrobenzene-d5	8.71	82	35166	4.37	ng	0.00
14) 2,4,6-Tribromophenol	15.67	330	20487	9.07	ng	-0.02
15) 2-Fluorobiphenyl	12.79	172	77455	4.27	ng	0.00
28) Terphenyl-d14	19.52	244	143814	6.17	ng	0.00
Target Compounds						
31) Bis(2-ethylhexyl)phthalate	21.00	149	1299	0.22	ng	Qvalue # 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091815\
Data File : BE090905.D
Acq On : 19 Sep 2015 10:31
Operator : UM/IZ
Sample : G3723-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
091615-D534-F-U-S

Quant Time: Sep 21 02:45:35 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 18 18:17:34 2015
Response via : Initial Calibration

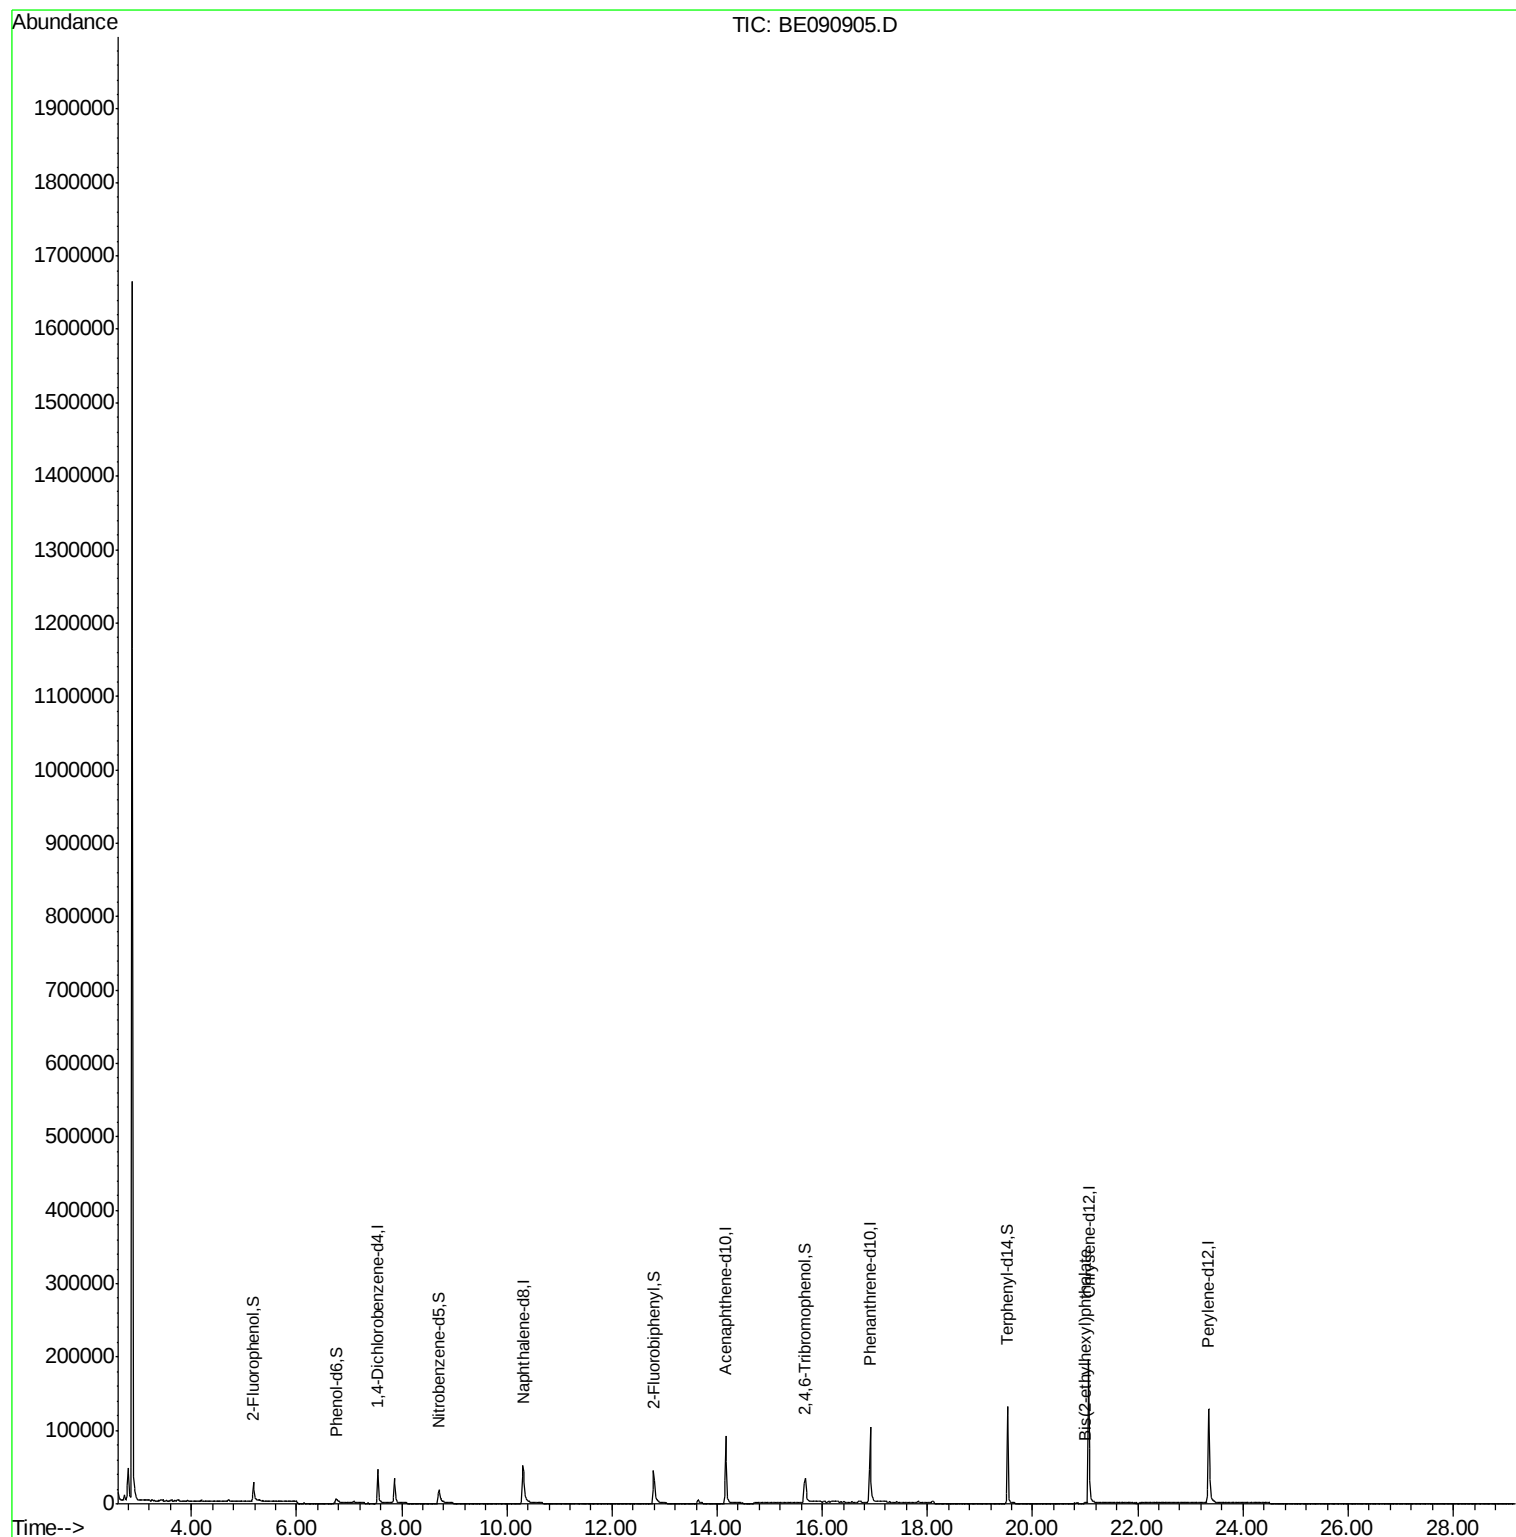

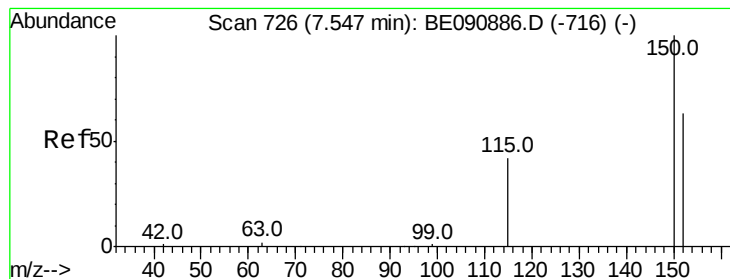

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.55 min Scan# 726

Delta R.T. -0.00 min

Lab File: BE090905.D

Acq: 19 Sep 2015 10:31

Instrument :

BNA_E

ClientSampleId :

091615-D534-F-U-S


Tgt Ion:152 Resp: 27272

Ion Ratio Lower Upper

152 100

150 158.1 122.2 183.4




115 69.6 51.0 76.4

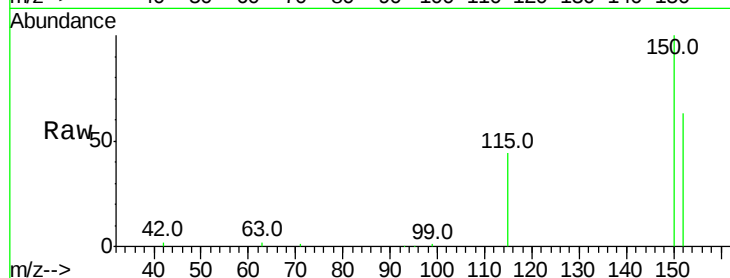

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

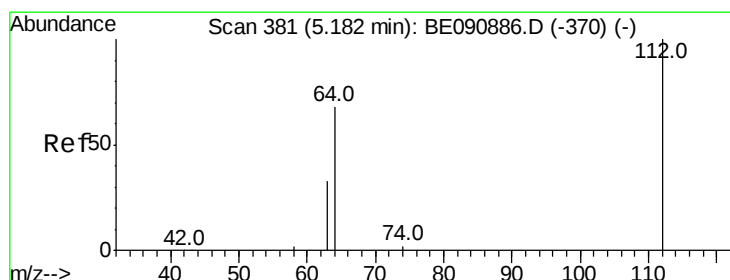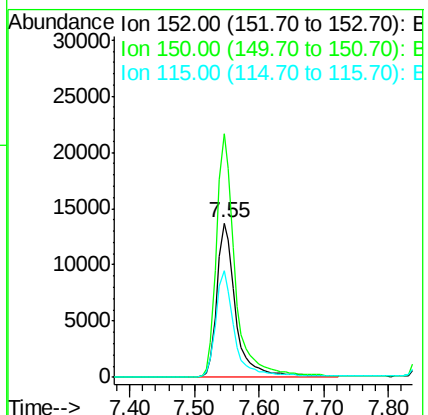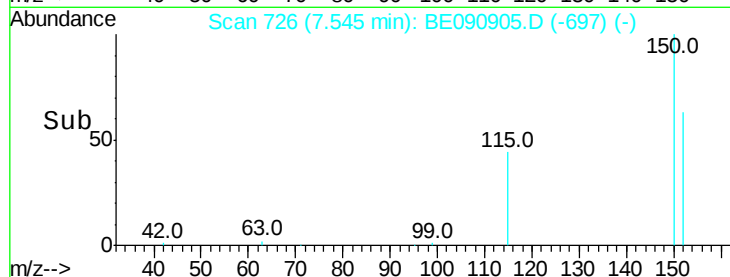

#4

2-Fluorophenol

Concen: 4.06 ng

RT: 5.18 min Scan# 380

Delta R.T. -0.01 min

Lab File: BE090905.D

Acq: 19 Sep 2015 10:31


Tgt Ion:112 Resp: 24923

Ion Ratio Lower Upper

112 100

64 72.8 57.3 85.9



63 36.8 29.2 43.8

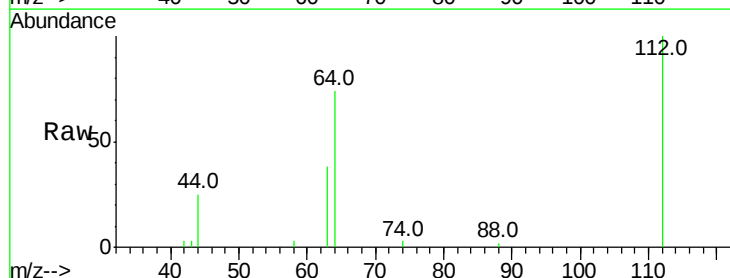


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

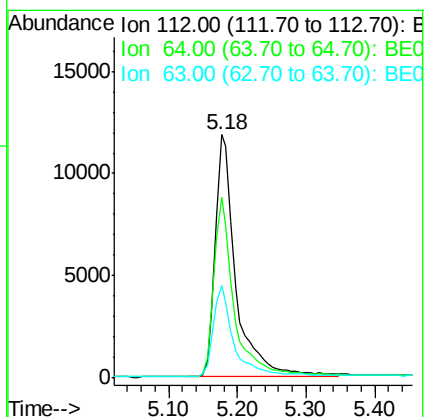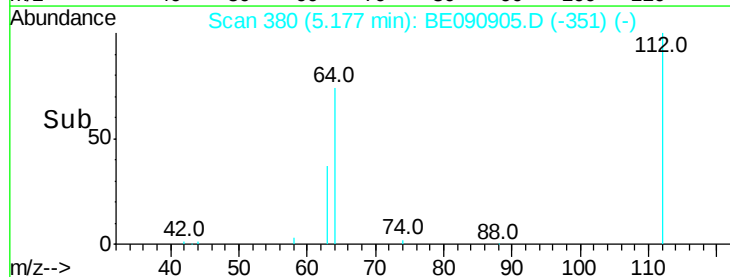



#5

Phenol-d6

Concen: 2.16 ng

RT: 6.75 min Scan# 609

Delta R.T. -0.00 min

Lab File: BE090905.D

Acq: 19 Sep 2015 10:31

Instrument :

BNA_E

ClientSampleId :

091615-D534-F-U-S





Tgt Ion: 99 Resp: 18325

Ion Ratio Lower Upper

99 100

42 21.8 16.8 25.2

71 36.3 28.3 42.5

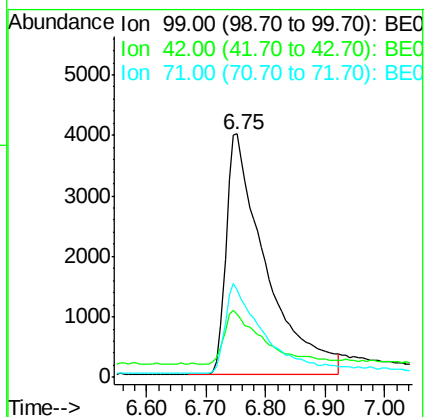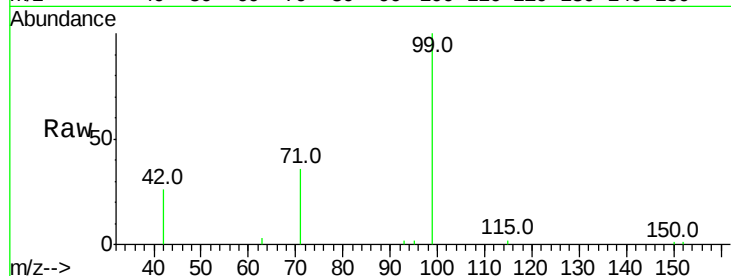

#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.31 min Scan# 1212

Delta R.T. 0.01 min

Lab File: BE090905.D

Acq: 19 Sep 2015 10:31

Tgt Ion: 136 Resp: 116673




Ion Ratio Lower Upper


136 100

137 11.4 8.7 13.1

54 11.3 9.0 13.6

68 8.1 6.3 9.5

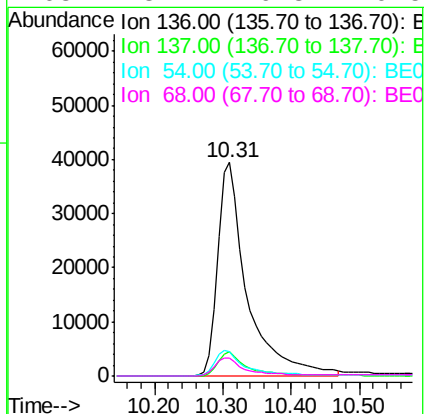

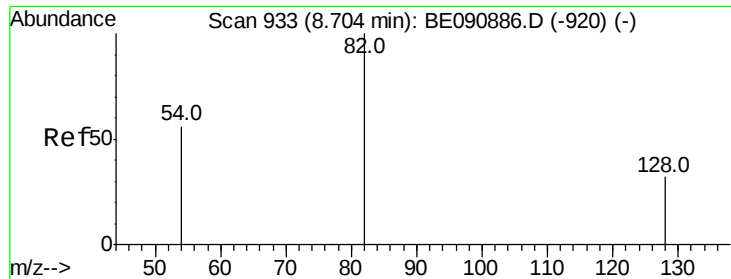

#8

Nitrobenzene-d5

Concen: 4.37 ng

RT: 8.71 min Scan# 934

Delta R.T. 0.01 min

Lab File: BE090905.D

Acq: 19 Sep 2015 10:31

Instrument :

BNA_E

ClientSampleId :

091615-D534-F-U-S


Tgt Ion: 82 Resp: 35166

Ion Ratio Lower Upper

82 100

128 30.5 25.0 37.4

54 57.4 46.3 69.5



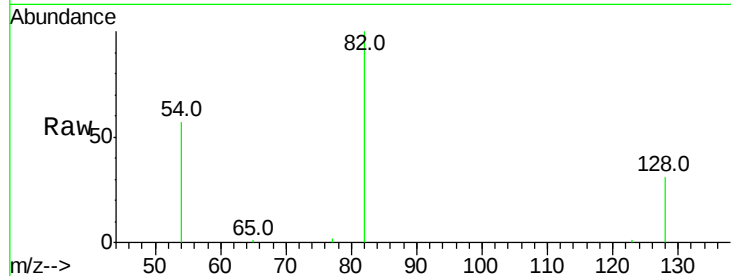


Abundance Ion 82.00 (81.70 to 82.70): BE090886.D (-920) (-)

Ion 128.00 (127.70 to 128.70): BE090886.D (-920) (-)

Ion 54.00 (53.70 to 54.70): BE090886.D (-920) (-)

Time-->

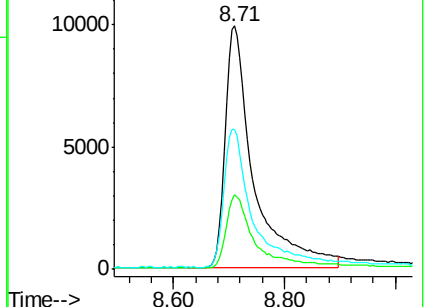

#13

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.16 min Scan# 1915

Delta R.T. -0.00 min

Lab File: BE090905.D

Acq: 19 Sep 2015 10:31


Tgt Ion: 164 Resp: 63993

Ion Ratio Lower Upper

164 100

162 106.2 86.8 130.2

160 58.4 53.9 80.9






Abundance Ion 164.00 (163.70 to 164.70): BE090886.D (-1907) (-)

Ion 162.00 (161.70 to 162.70): BE090886.D (-1907) (-)

Ion 160.00 (159.70 to 160.70): BE090886.D (-1907) (-)

Time-->

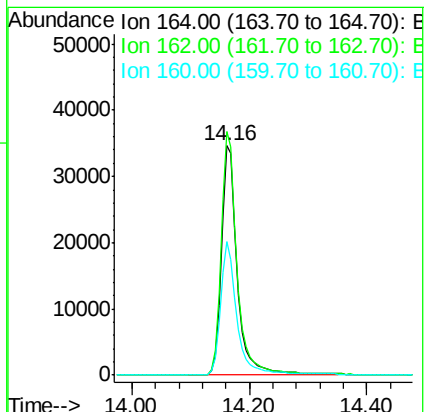


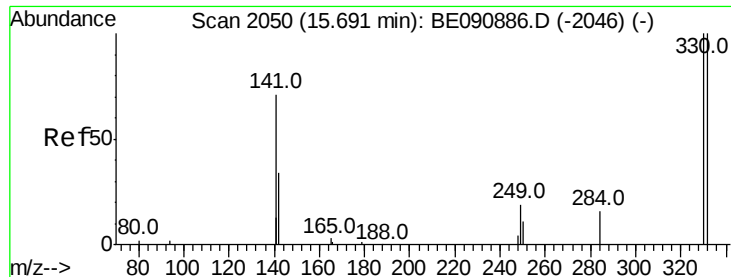




#14
 2,4,6-Tribromophenol
 Concen: 9.07 ng
 RT: 15.67 min Scan# 2050
 Delta R.T. -0.02 min
 Lab File: BE090905.D
 Acq: 19 Sep 2015 10:31

Instrument :
 BNA_E
 ClientSampleId :
 091615-D534-F-U-S

Tgt Ion: 330 Resp: 20487
 Ion Ratio Lower Upper
 330 100
 332 97.3 74.9 112.3
 141 178.0 145.2 217.8

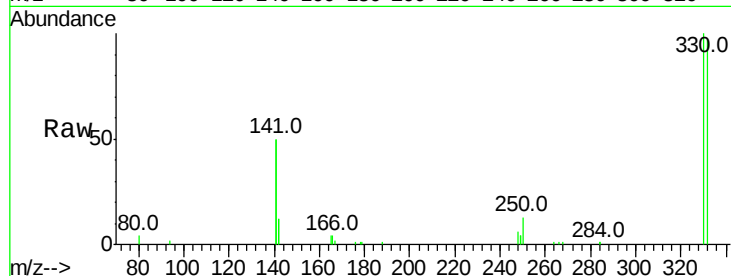


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

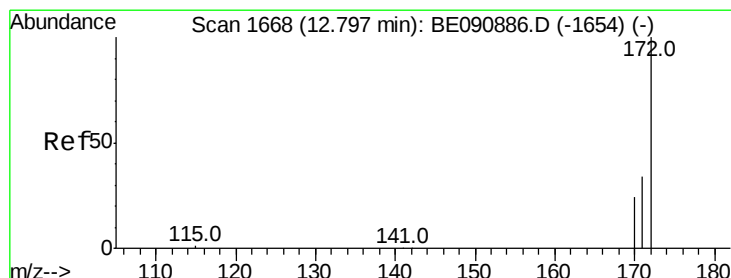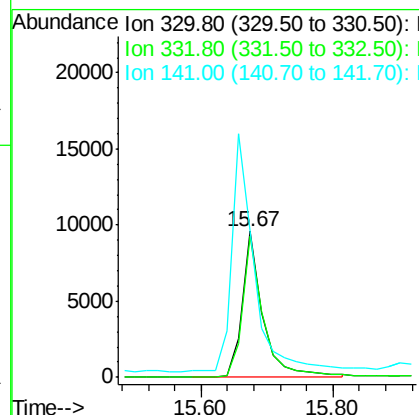




#15
 2-Fluorobiphenyl
 Concen: 4.27 ng
 RT: 12.79 min Scan# 1667
 Delta R.T. -0.01 min
 Lab File: BE090905.D
 Acq: 19 Sep 2015 10:31

Tgt Ion: 172 Resp: 77455
 Ion Ratio Lower Upper
 172 100
 171 34.4 27.8 41.8
 170 24.0 19.8 29.6



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

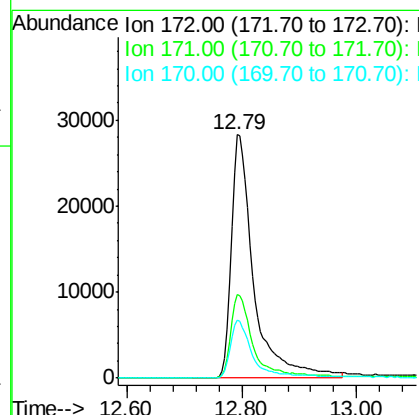



#19

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.91 min Scan# 2121

Delta R.T. 0.00 min

Lab File: BE090905.D

Acq: 19 Sep 2015 10:31

Instrument :

BNA_E

ClientSampleId :

091615-D534-F-U-S


Tgt Ion:188 Resp: 154143

Ion Ratio Lower Upper

188 100

94 9.4 10.3 15.5#




80 9.9 11.0 16.6#

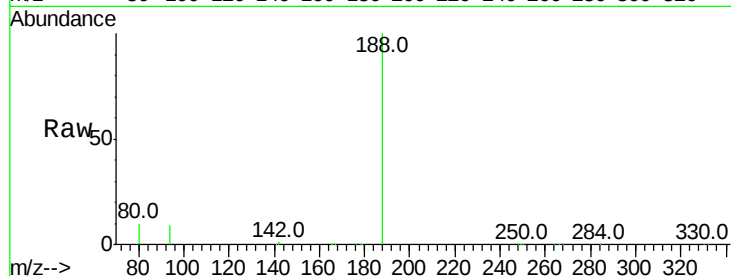

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

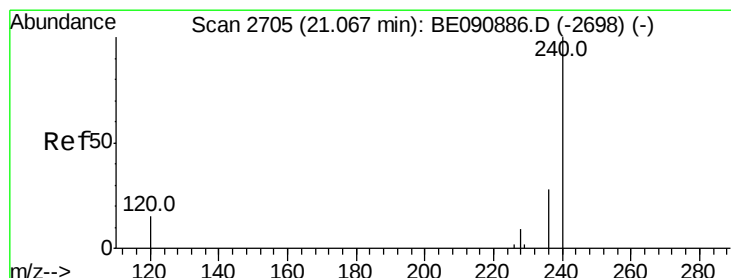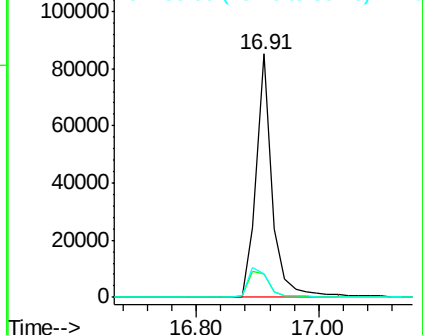

#26

Chrysene-d12

Concen: 5.00 ng

RT: 21.07 min Scan# 2705

Delta R.T. -0.00 min

Lab File: BE090905.D

Acq: 19 Sep 2015 10:31


Tgt Ion:240 Resp: 206505

Ion Ratio Lower Upper

240 100

120 13.6 10.1 15.1



236 27.2 21.9 32.9

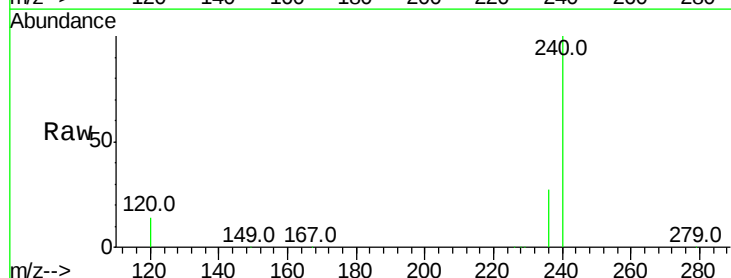


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

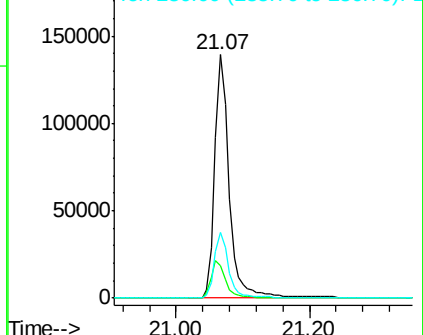

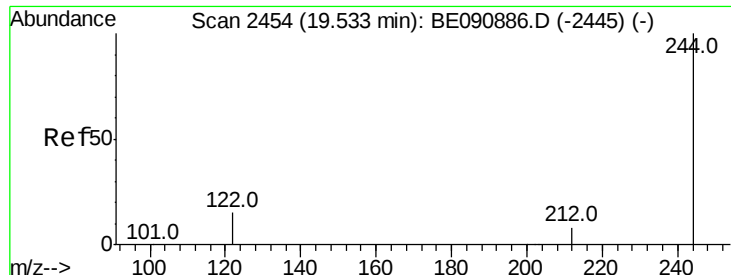

#28

Terphenyl-d14

Concen: 6.17 ng

RT: 19.52 min Scan# 2453

Delta R.T. -0.01 min

Lab File: BE090905.D

Acq: 19 Sep 2015 10:31

Instrument :

BNA_E

ClientSampleId :

091615-D534-F-U-S


Tgt Ion:244 Resp: 143814

Ion Ratio Lower Upper

244 100

212 8.6 6.9 10.3




122 15.9 12.9 19.3

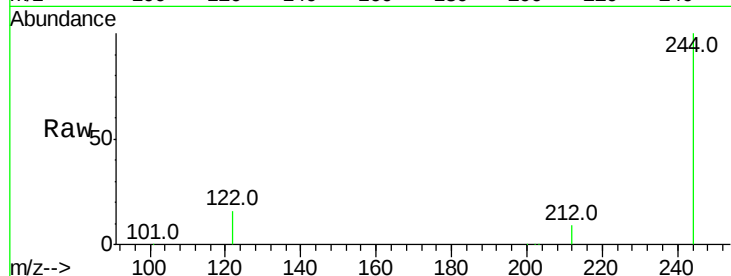

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

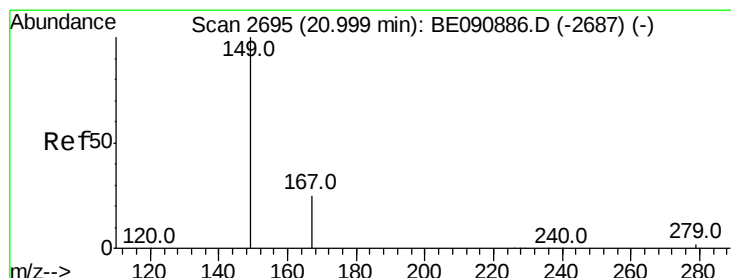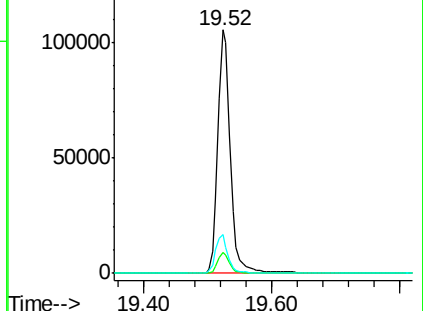

#31

Bis(2-ethylhexyl)phthalate

Concen: 0.22 ng

RT: 21.00 min Scan# 2695

Delta R.T. -0.00 min

Lab File: BE090905.D

Acq: 19 Sep 2015 10:31


Tgt Ion:149 Resp: 1299

Ion Ratio Lower Upper

149 100

167 23.5 20.1 30.1



279 4.2 2.3 3.5#




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

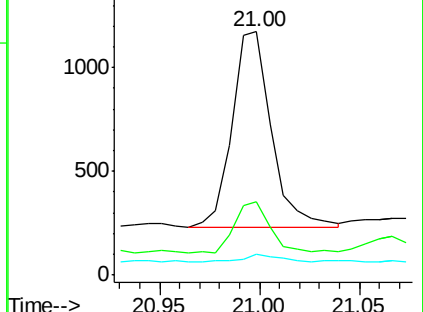

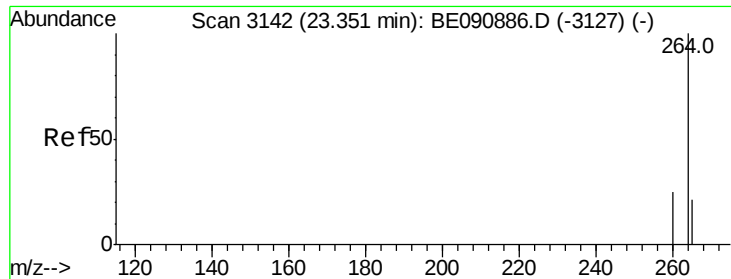

#33

Perylene-d12

Concen: 5.00 ng

RT: 23.35 min Scan# 3142

Delta R.T. -0.00 min

Lab File: BE090905.D


Acq: 19 Sep 2015 10:31

Instrument :

BNA_E

ClientSampleId :

091615-D534-F-U-S

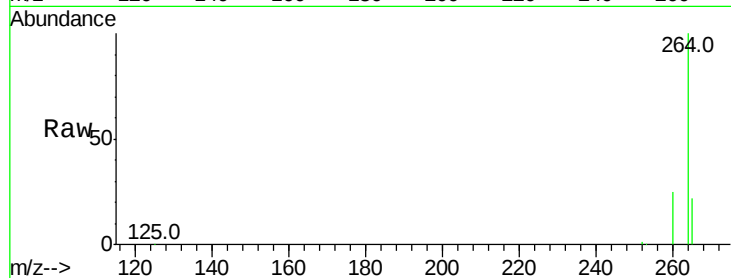


Tgt Ion: 264 Resp: 199466

Ion Ratio Lower Upper

264 100

260 25.2 19.7 29.5

265 21.5 17.5 26.3

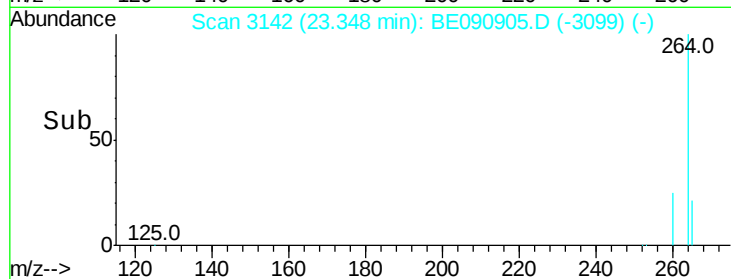

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

