

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091815\
 Data File : BE090906.D
 Acq On : 19 Sep 2015 11:07
 Operator : UM/IZ
 Sample : G3723-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 091615-D534-F-D-B

Quant Time: Sep 21 02:47:13 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 18 18:17:34 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	23668	5.00	ng	0.00
7) Naphthalene-d8	10.31	136	98885	5.00	ng	0.00
13) Acenaphthene-d10	14.17	164	53258	5.00	ng	0.00
19) Phenanthrene-d10	16.91	188	133875	5.00	ng	0.00
26) Chrysene-d12	21.07	240	181913	5.00	ng	0.00
33) Perylene-d12	23.35	264	173959	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.18	112	19274	3.61	ng	0.00
5) Phenol-d6	6.75	99	14209	1.93	ng	0.00
8) Nitrobenzene-d5	8.71	82	28915	4.24	ng	0.00
14) 2,4,6-Tribromophenol	15.67	330	16927	9.00	ng	-0.02
15) 2-Fluorobiphenyl	12.80	172	64806	4.29	ng	0.00
28) Terphenyl-d14	19.53	244	128451	6.26	ng	0.00
Target Compounds						
31) Bis(2-ethylhexyl)phthalate	21.00	149	1372	0.23	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091815\
Data File : BE090906.D
Acq On : 19 Sep 2015 11:07
Operator : UM/IZ
Sample : G3723-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
091615-D534-F-D-B

Quant Time: Sep 21 02:47:13 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 18 18:17:34 2015
Response via : Initial Calibration

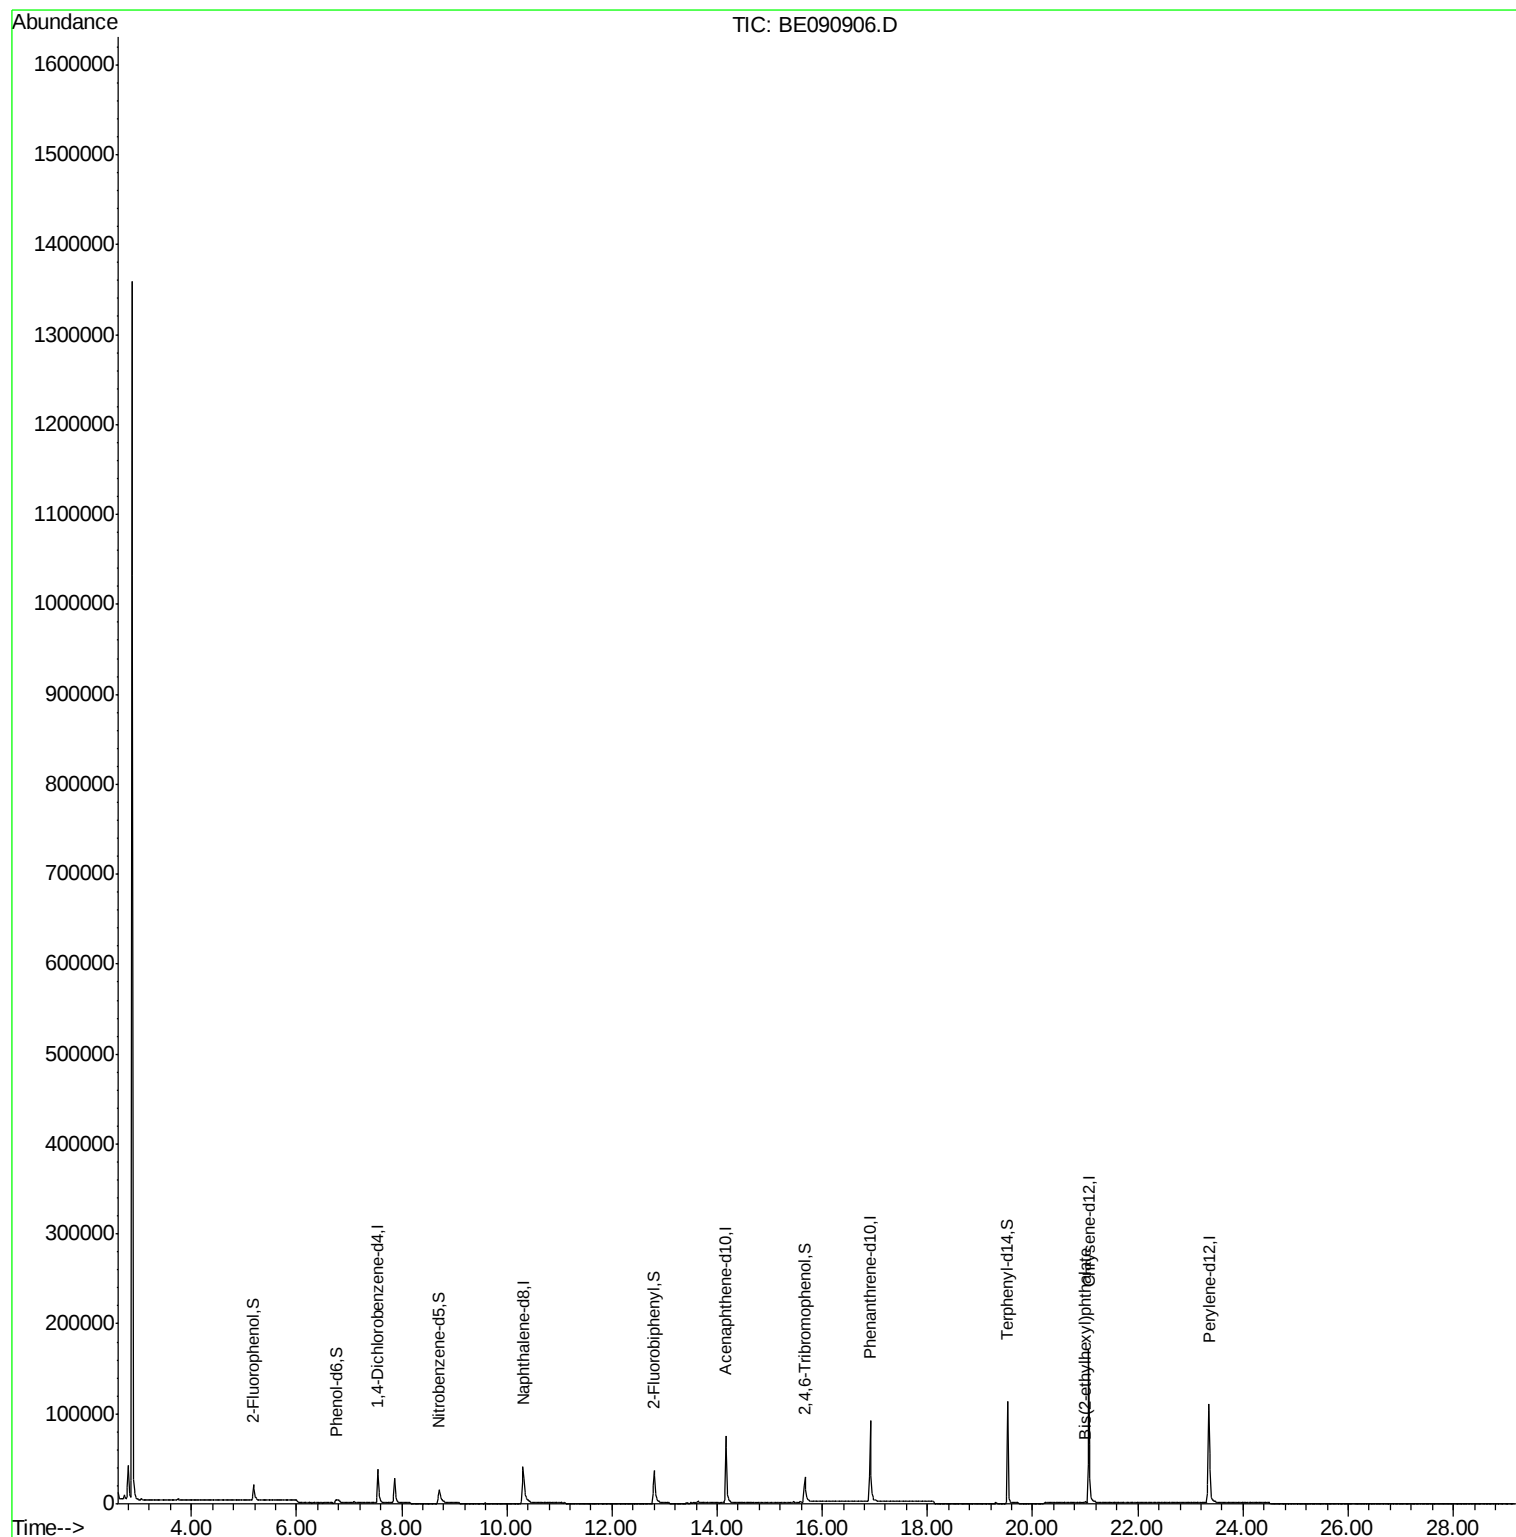


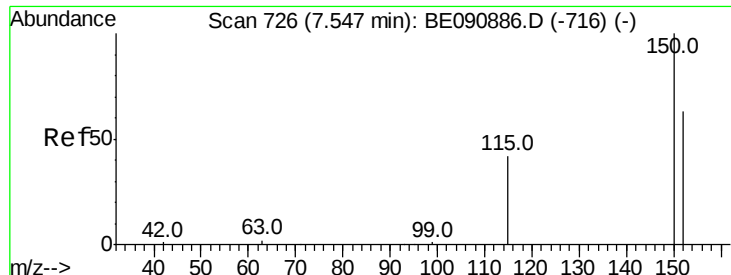




#1
 1,4-Dichlorobenzene-d4
 Concen: 5.00 ng
 RT: 7.55 min Scan# 726
 Delta R.T. 0.00 min
 Lab File: BE090906.D
 Acq: 19 Sep 2015 11:07

Instrument :
 BNA_E
 ClientSampleId :
 091615-D534-F-D-B

Tgt Ion:152 Resp: 23668
 Ion Ratio Lower Upper
 152 100
 150 156.1 122.2 183.4
 115 68.1 51.0 76.4

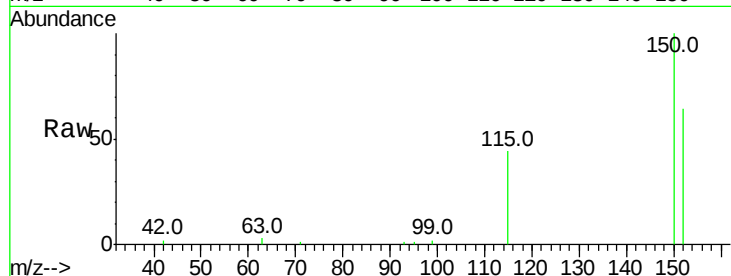


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

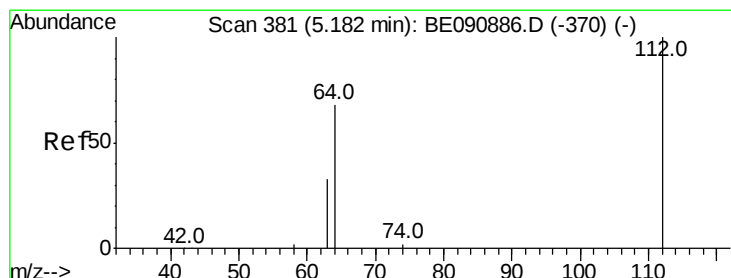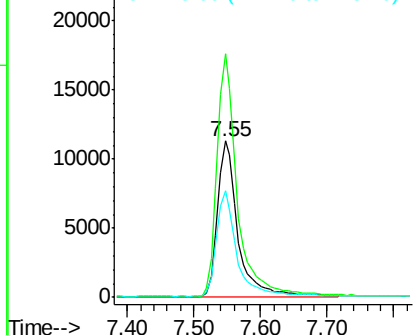
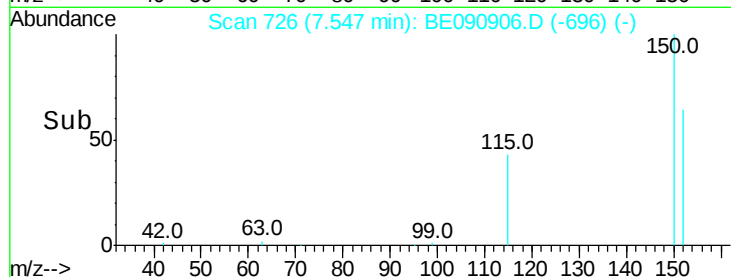



#4
 2-Fluorophenol
 Concen: 3.61 ng
 RT: 5.18 min Scan# 381
 Delta R.T. 0.00 min
 Lab File: BE090906.D
 Acq: 19 Sep 2015 11:07

Tgt Ion:112 Resp: 19274
 Ion Ratio Lower Upper
 112 100
 64 71.2 57.3 85.9
 63 36.7 29.2 43.8

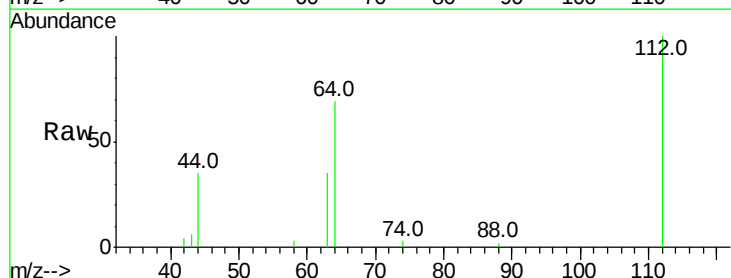

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BE0
 Ion 63.00 (62.70 to 63.70): BE0

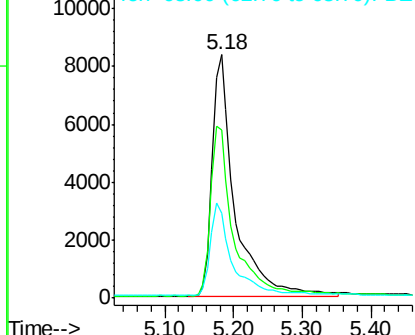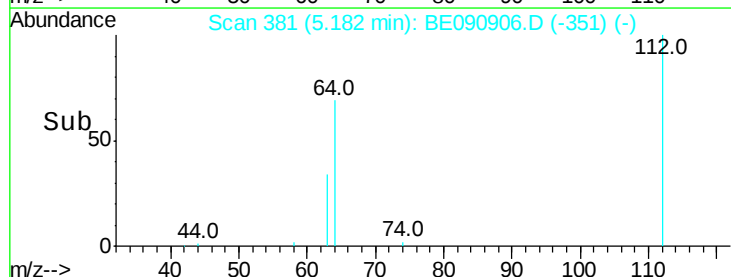

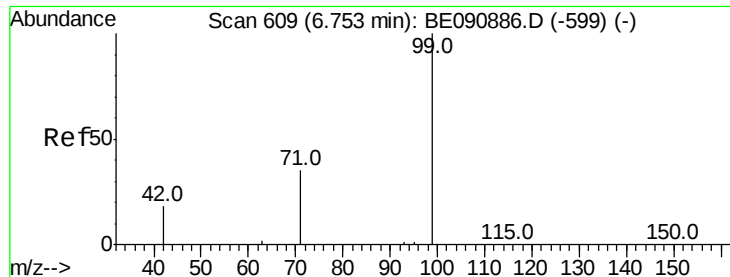

#5

Phenol-d6

Concen: 1.93 ng

RT: 6.75 min Scan# 609

Delta R.T. 0.00 min

Lab File: BE090906.D

Acq: 19 Sep 2015 11:07

Instrument :

BNA_E

ClientSampleId :

091615-D534-F-D-B


Tgt Ion: 99 Resp: 14209

Ion Ratio Lower Upper

99 100

42 20.9 16.8 25.2




71 36.4 28.3 42.5

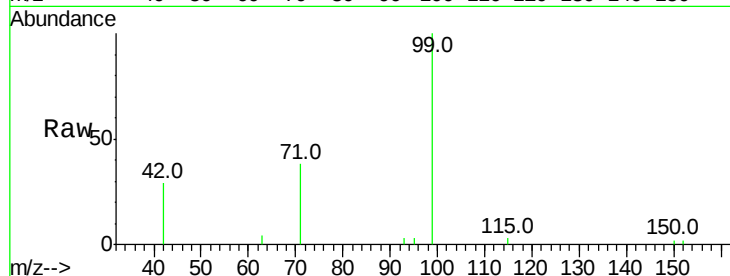

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

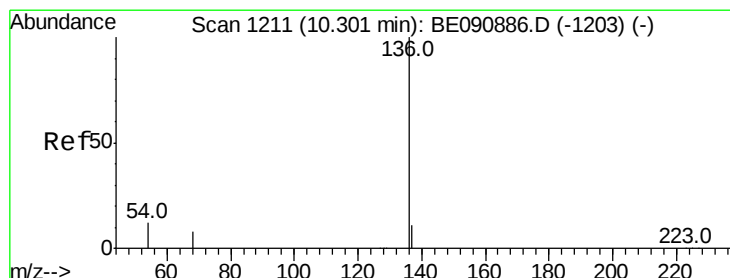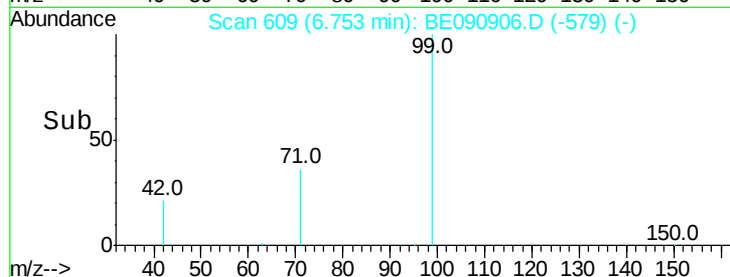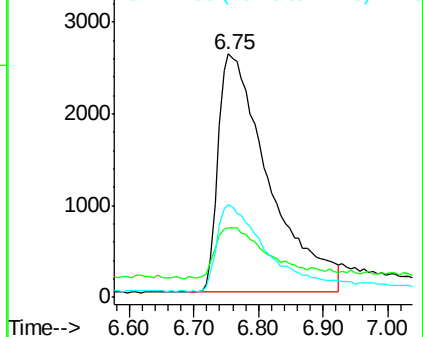

#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.31 min Scan# 1212

Delta R.T. 0.01 min

Lab File: BE090906.D

Acq: 19 Sep 2015 11:07

Tgt Ion: 136 Resp: 98885


Ion Ratio Lower Upper

136 100

137 10.9 8.7 13.1

54 11.9 9.0 13.6

68 8.5 6.3 9.5


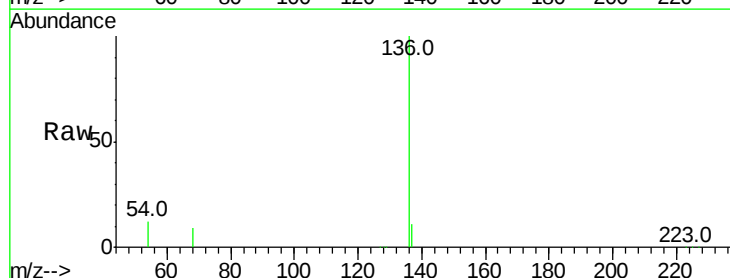



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

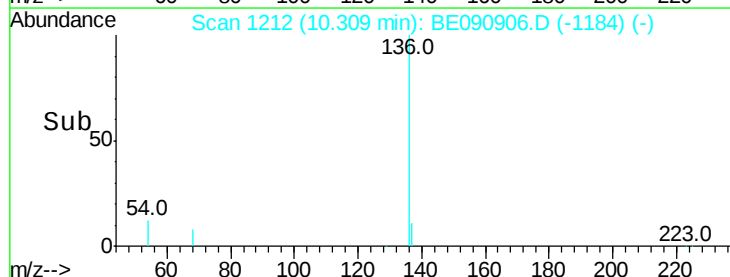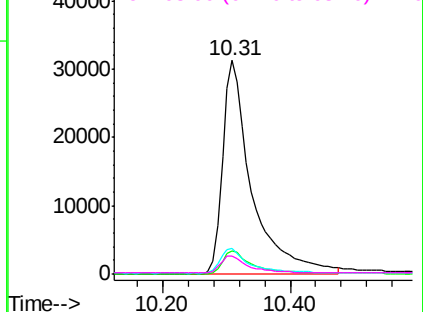

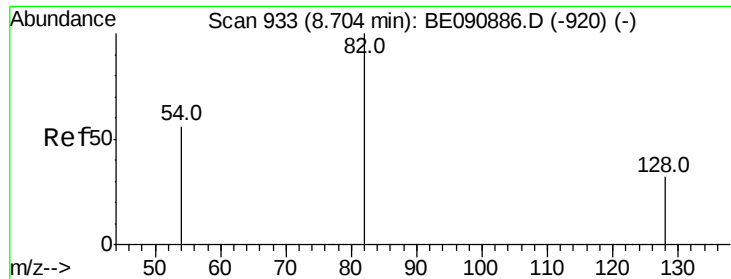

#8

Nitrobenzene-d5

Concen: 4.24 ng

RT: 8.71 min Scan# 935

Delta R.T. 0.01 min

Lab File: BE090906.D

Acq: 19 Sep 2015 11:07

Instrument :

BNA_E

ClientSampleId :

091615-D534-F-D-B


Tgt Ion: 82 Resp: 28915

Ion Ratio Lower Upper

82 100

128 30.3 25.0 37.4




54 58.2 46.3 69.5

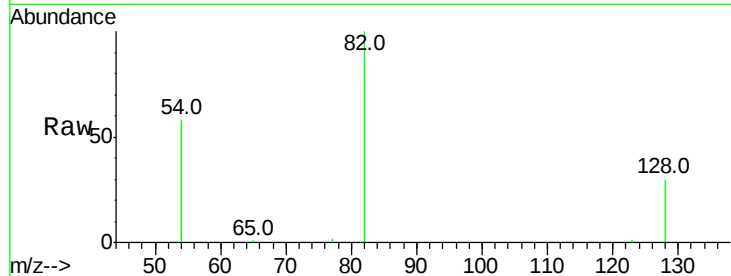

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

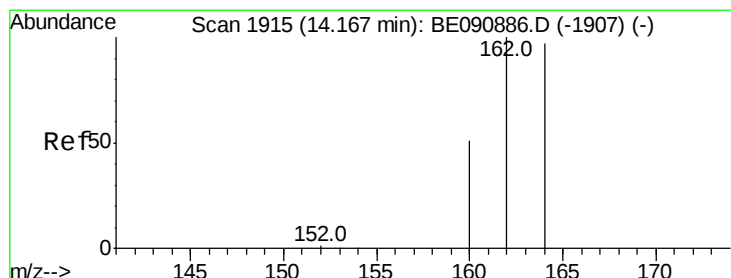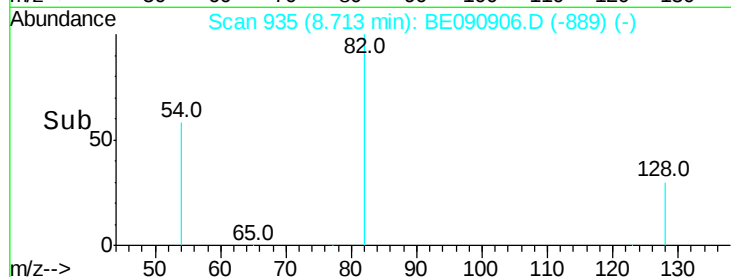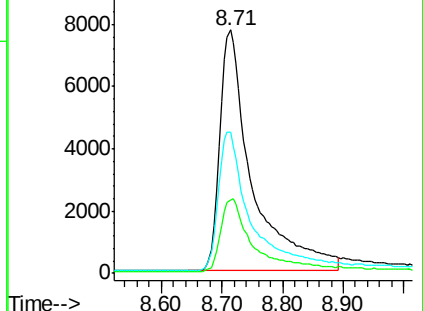

#13

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.17 min Scan# 1915

Delta R.T. 0.00 min

Lab File: BE090906.D

Acq: 19 Sep 2015 11:07


Tgt Ion: 164 Resp: 53258

Ion Ratio Lower Upper

164 100

162 106.4 86.8 130.2



160 58.1 53.9 80.9

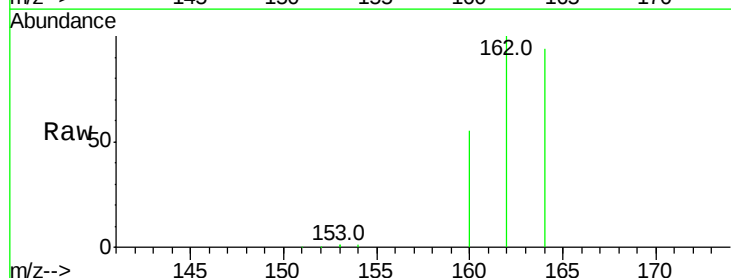


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

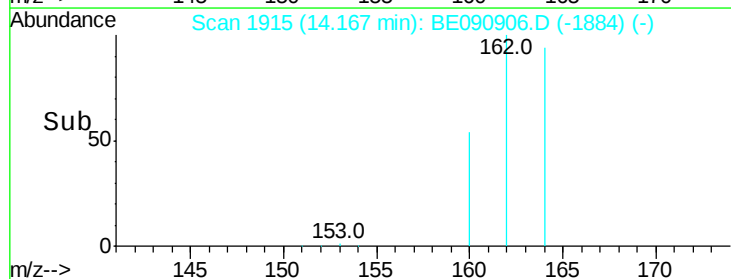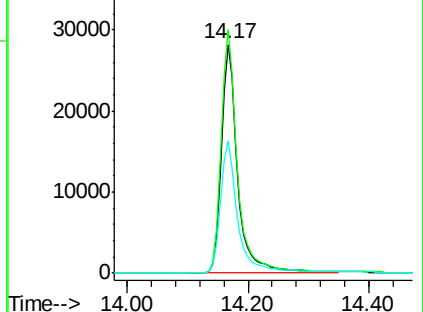


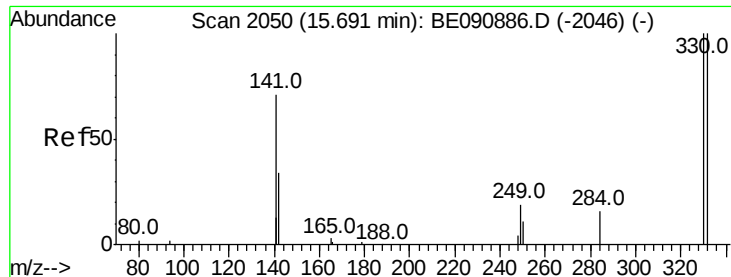




#14
 2,4,6-Tribromophenol
 Concen: 9.00 ng
 RT: 15.67 min Scan# 2049
 Delta R.T. -0.02 min
 Lab File: BE090906.D
 Acq: 19 Sep 2015 11:07

Instrument :
 BNA_E
 ClientSampleId :
 091615-D534-F-D-B

Tgt Ion: 330 Resp: 16927
 Ion Ratio Lower Upper
 330 100
 332 97.5 74.9 112.3
 141 175.3 145.2 217.8

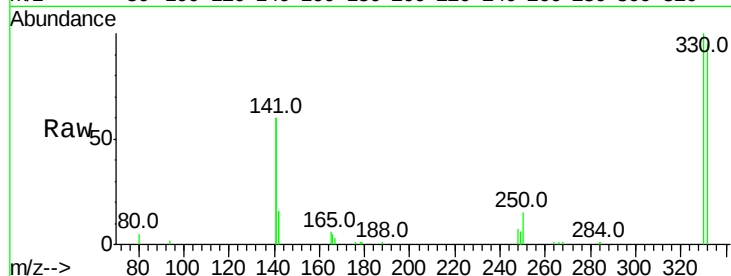


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

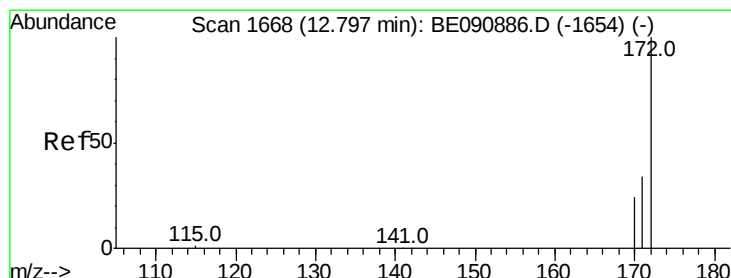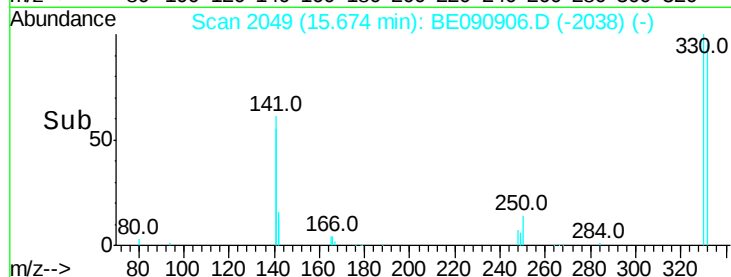
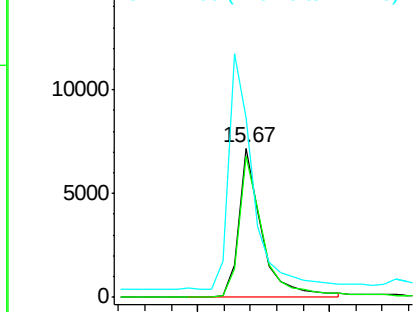



#15
 2-Fluorobiphenyl
 Concen: 4.29 ng
 RT: 12.80 min Scan# 1668
 Delta R.T. 0.00 min
 Lab File: BE090906.D
 Acq: 19 Sep 2015 11:07

Tgt Ion: 172 Resp: 64806
 Ion Ratio Lower Upper
 172 100
 171 34.9 27.8 41.8
 170 24.2 19.8 29.6

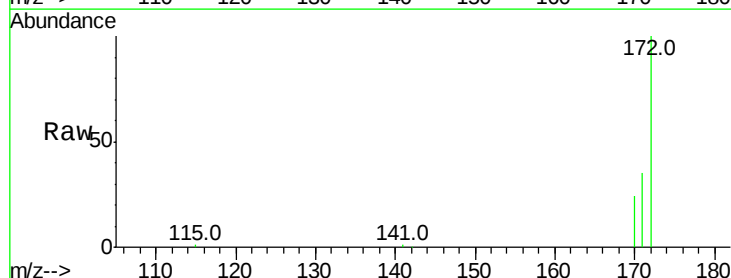

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

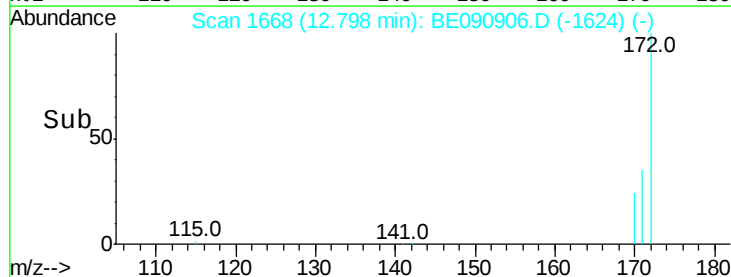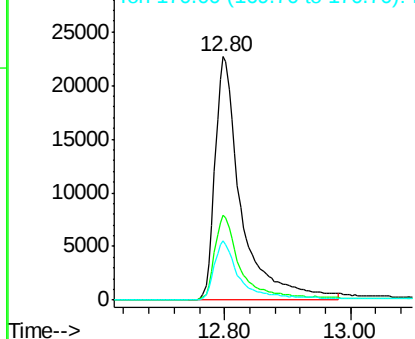

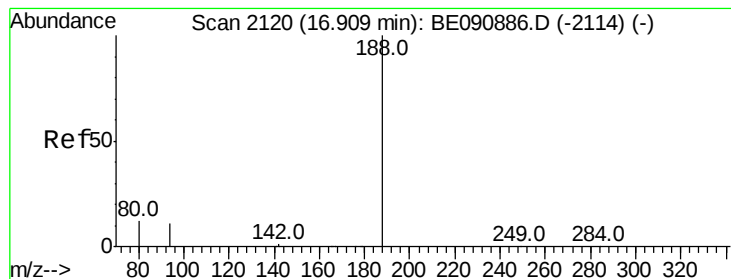

#19

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.91 min Scan# 2120

Delta R.T. 0.00 min

Lab File: BE090906.D

Acq: 19 Sep 2015 11:07

Instrument :

BNA_E

ClientSampleId :

091615-D534-F-D-B


Tgt Ion:188 Resp: 133875

Ion Ratio Lower Upper

188 100

94 10.2 10.3 15.5#




80 11.2 11.0 16.6

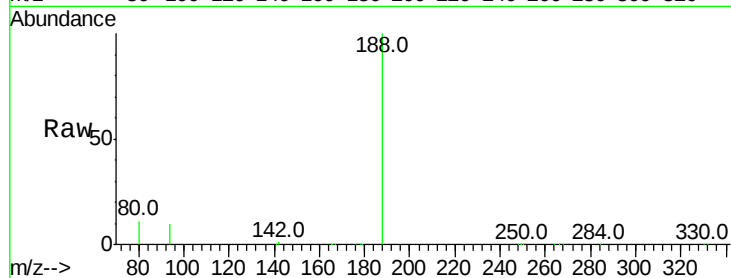

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

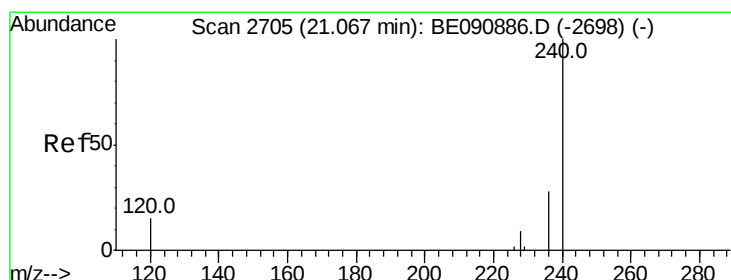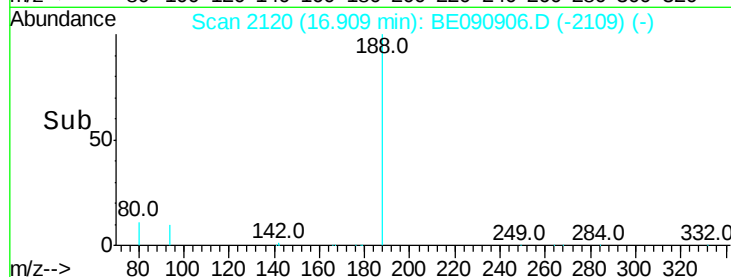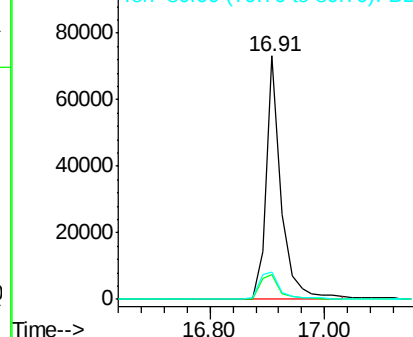

#26

Chrysene-d12

Concen: 5.00 ng

RT: 21.07 min Scan# 2705

Delta R.T. 0.00 min

Lab File: BE090906.D

Acq: 19 Sep 2015 11:07


Tgt Ion:240 Resp: 181913

Ion Ratio Lower Upper

240 100

120 14.0 10.1 15.1



236 27.7 21.9 32.9

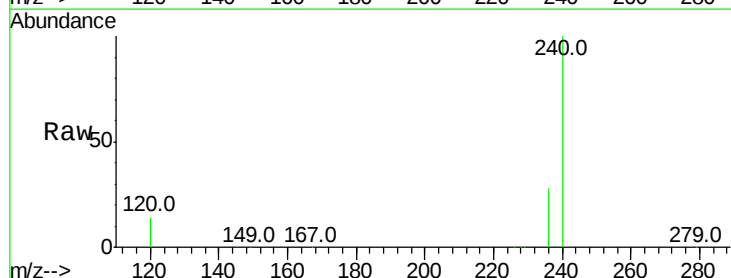


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

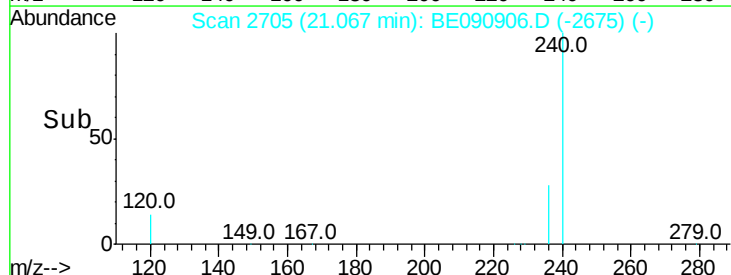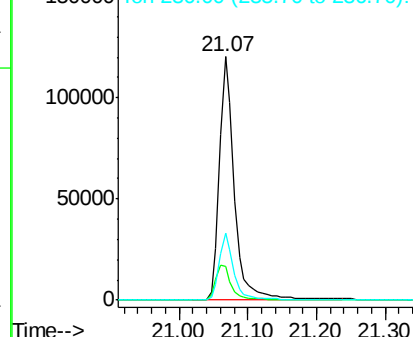

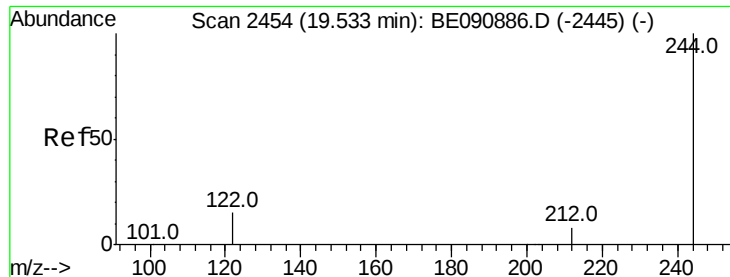

#28

Terphenyl-d14

Concen: 6.26 ng

RT: 19.53 min Scan# 2453

Delta R.T. -0.00 min

Lab File: BE090906.D

Acq: 19 Sep 2015 11:07

Instrument :

BNA_E

ClientSampleId :

091615-D534-F-D-B


Tgt Ion:244 Resp: 128451

Ion Ratio Lower Upper

244 100

212 8.1 6.9 10.3




122 12.8 12.9 19.3#

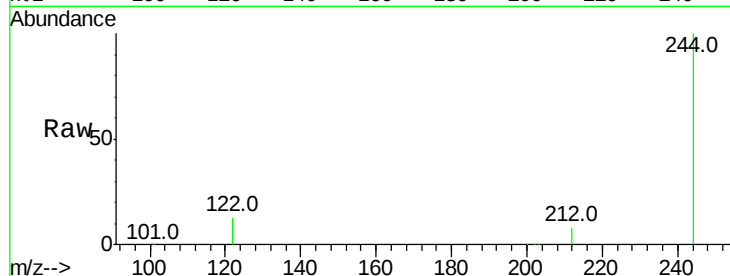

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

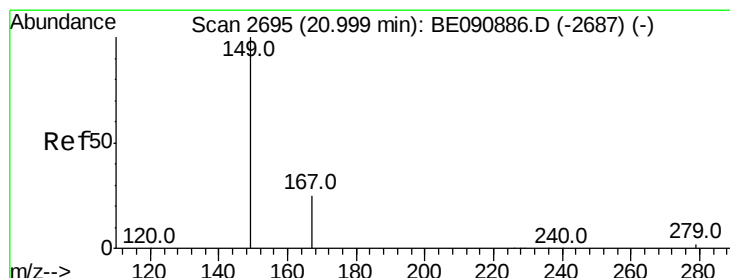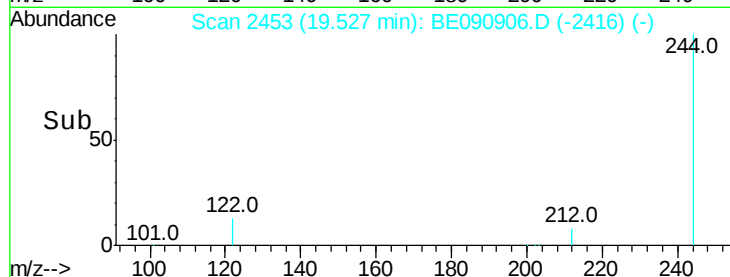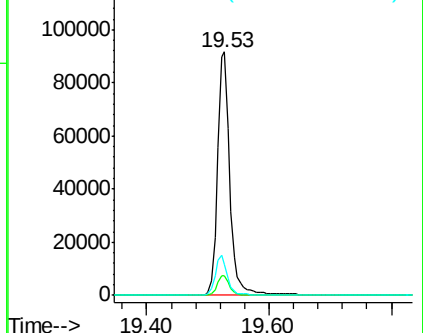

#31

Bis(2-ethylhexyl)phthalate

Concen: 0.23 ng

RT: 21.00 min Scan# 2695

Delta R.T. 0.00 min

Lab File: BE090906.D

Acq: 19 Sep 2015 11:07


Tgt Ion:149 Resp: 1372

Ion Ratio Lower Upper

149 100

167 23.5 20.1 30.1



279 3.4 2.3 3.5



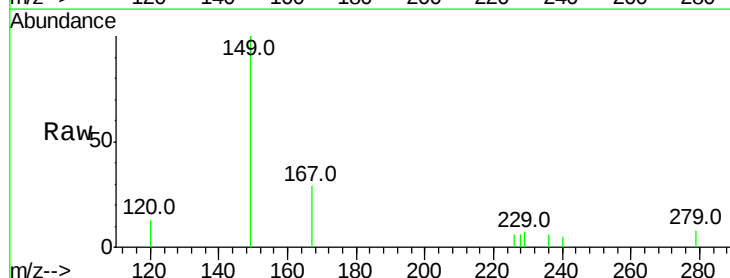


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

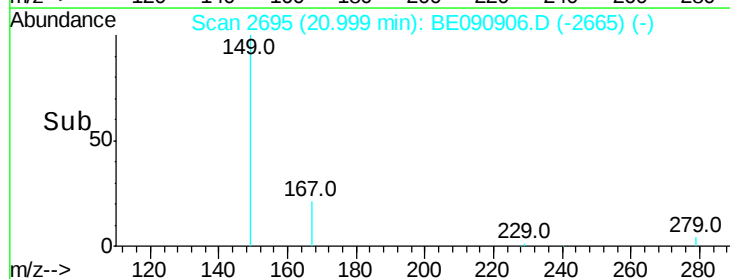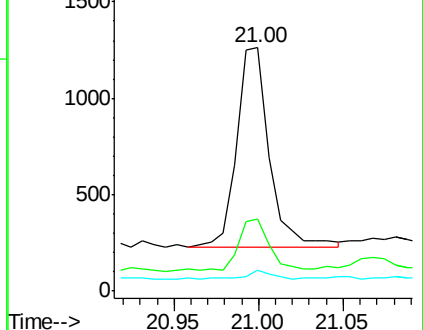

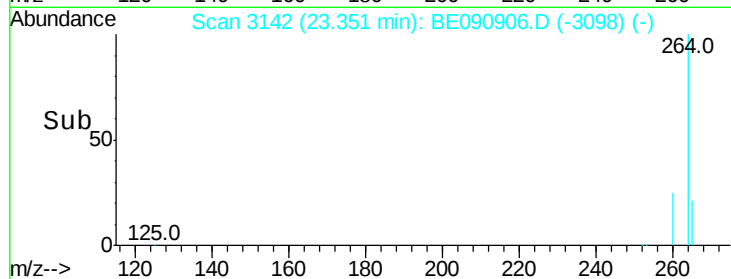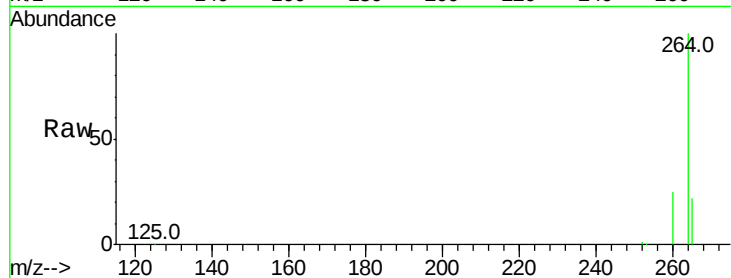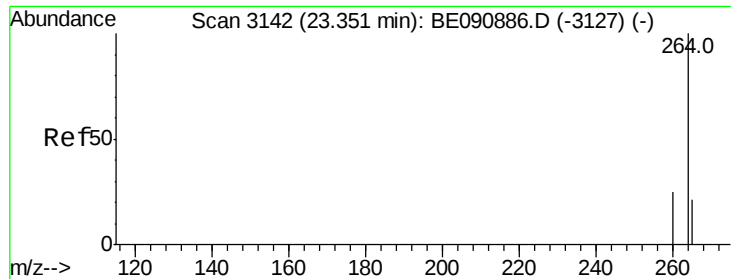

#33

Perylene-d12

Concen: 5.00 ng

RT: 23.35 min Scan# 3142

Delta R.T. 0.00 min

Lab File: BE090906.D

Acq: 19 Sep 2015 11:07

Instrument :

BNA_E

ClientSampleId :

091615-D534-F-D-B

Tgt Ion:264 Resp: 173959

Ion Ratio Lower Upper

264 100

260 25.2 19.7 29.5

265 22.0 17.5 26.3

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

