


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091815\
Data File : BE090881.D
Acq On : 18 Sep 2015 9:33
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 18 18:17:34 2015

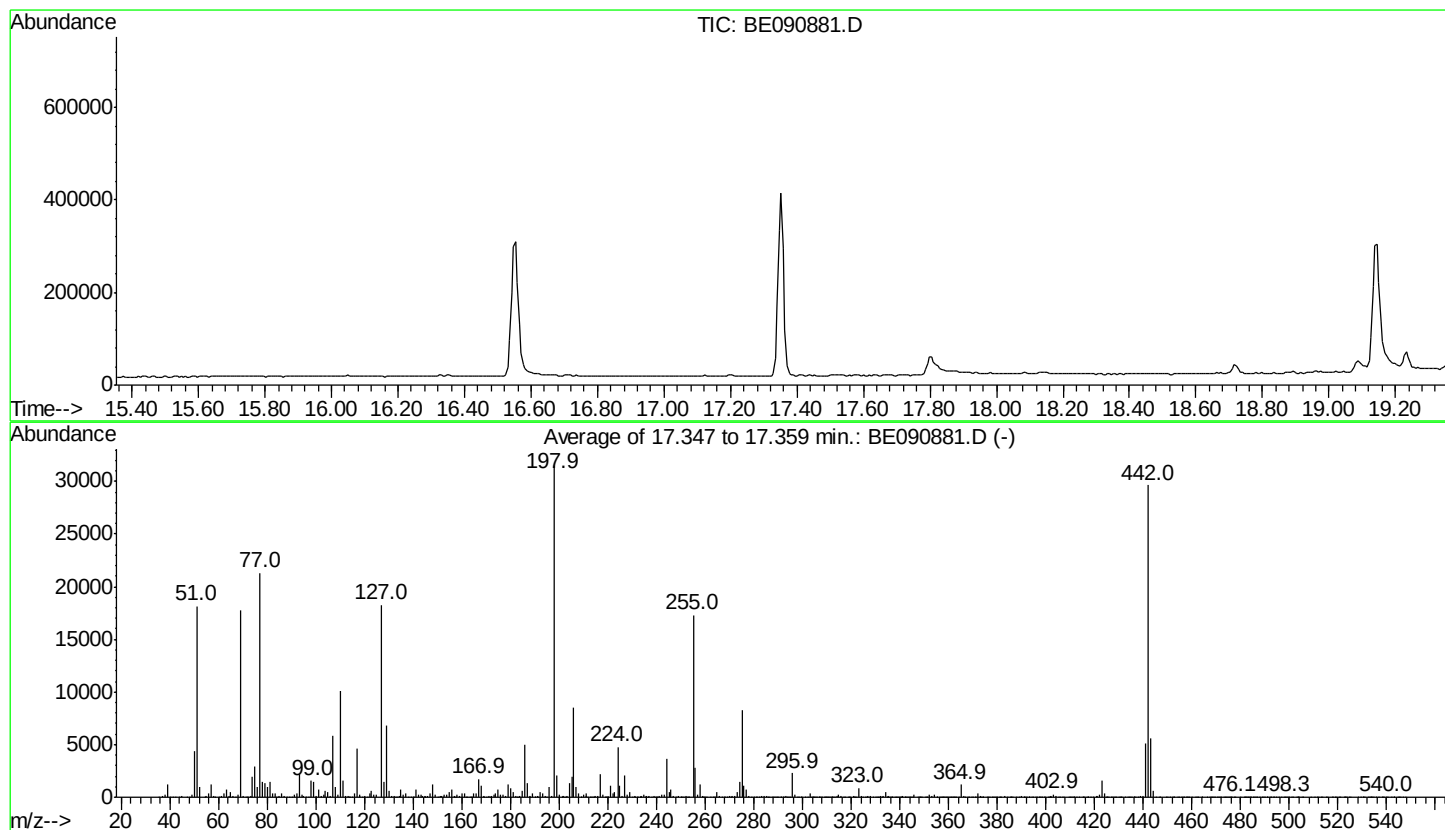

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.6	18155	PASS
68	69	0.00	2	1.1	193	PASS
69	198	0.00	100	56.2	17702	PASS
70	69	0.00	2	0.5	84	PASS
127	198	10	80	58.0	18261	PASS
197	198	0.00	2	0.3	86	PASS
198	198	100	100	100.0	31501	PASS
199	198	5	9	6.7	2120	PASS
275	198	10	60	26.3	8285	PASS
365	198	1	100	3.8	1186	PASS
441	442	0.01	24	17.3	5136	PASS
442	198	50	100	94.2	29664	PASS
443	442	15	24	18.9	5607	PASS