


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE091815\
 Data File : BE090891.D
 Acq On : 18 Sep 2015 23:26
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 18 18:17:34 2015

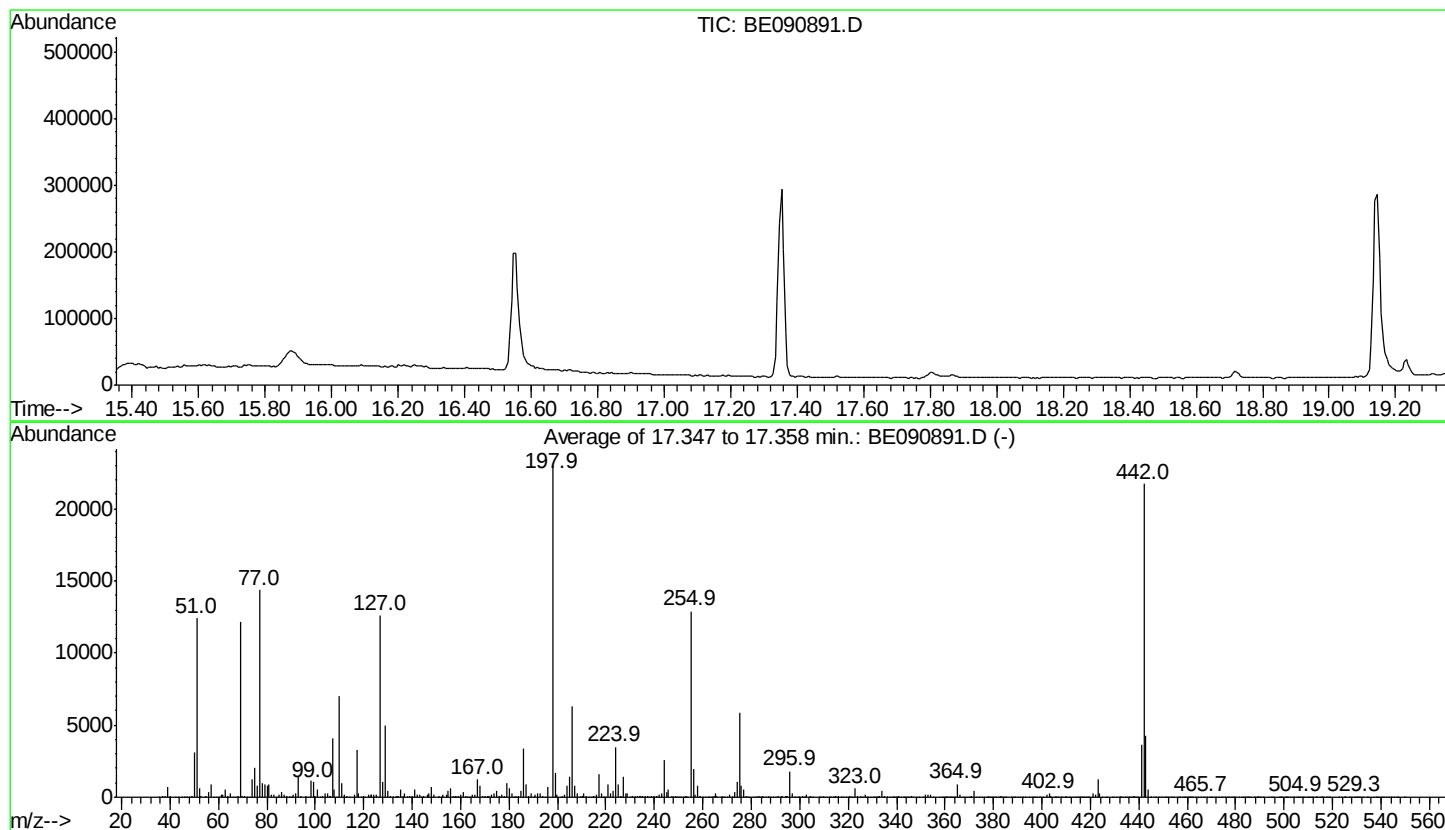

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.9	12396	PASS
68	69	0.00	2	0.7	82	PASS
69	198	0.00	100	52.8	12136	PASS
70	69	0.00	2	0.8	101	PASS
127	198	10	80	54.7	12571	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22992	PASS
199	198	5	9	7.5	1723	PASS
275	198	10	60	25.4	5841	PASS
365	198	1	100	3.9	888	PASS
441	442	0.01	24	16.9	3675	PASS
442	198	50	100	94.5	21725	PASS
443	442	15	24	19.5	4235	PASS