
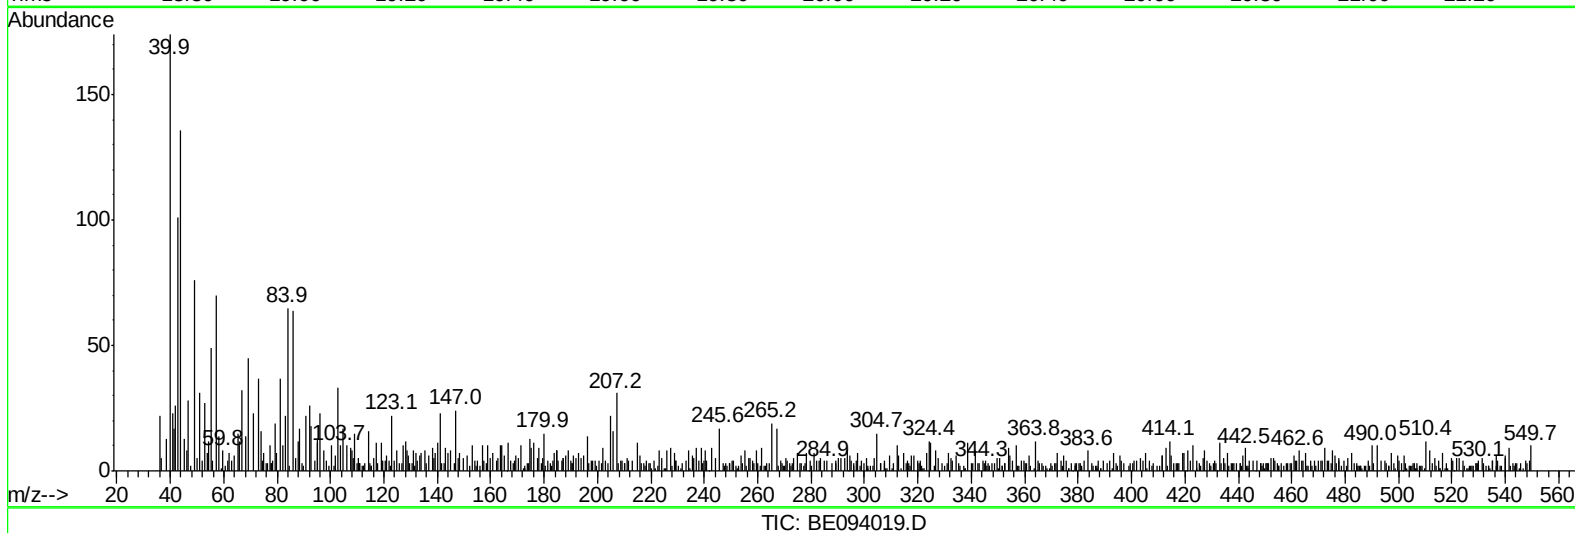


Data Path : Z:\HPCHEM1\BNA E\DATA\BE091817\
Data File : BE094019.D
Acq On : 18 Sep 2017 10:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 02:09:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 18 13:37:24 2017
Response via : Initial Calibration

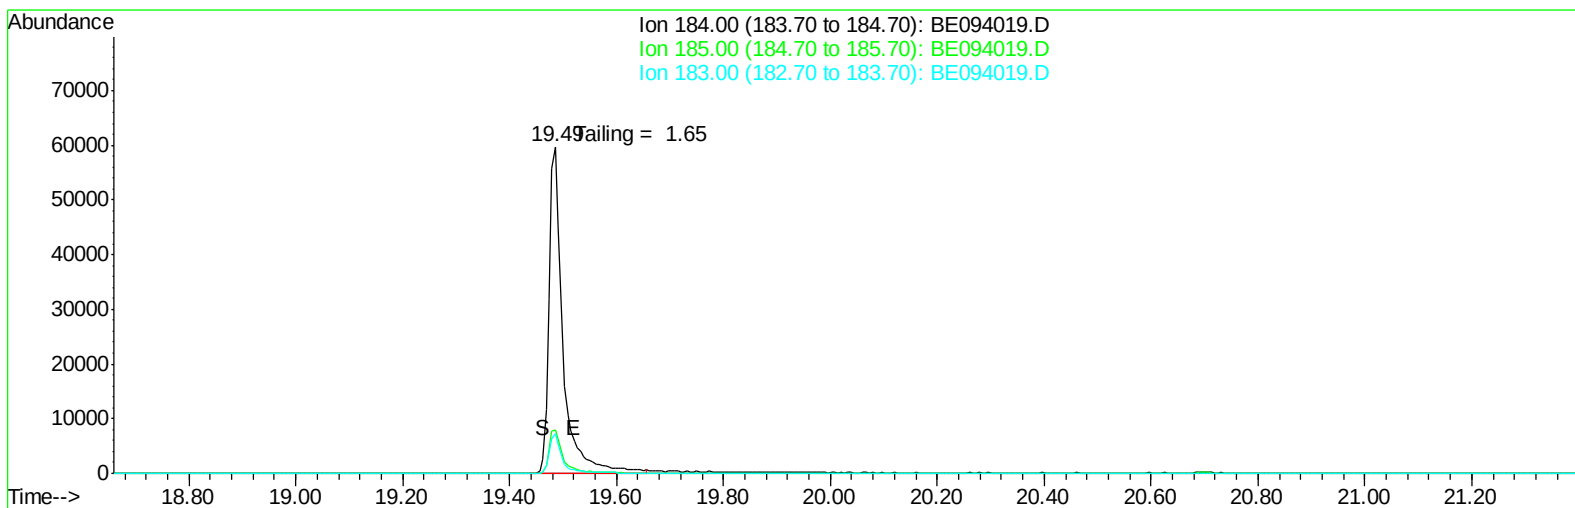

TIC: BE094019.D

(76) Benzidine



12.511min (+0.025) 8.32ng

response 7

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	80.00#
183.00	12.20	40.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE091817\
Data File : BE094019.D
Acq On : 18 Sep 2017 10:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 02:09:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 18 13:37:24 2017
Response via : Initial Calibration

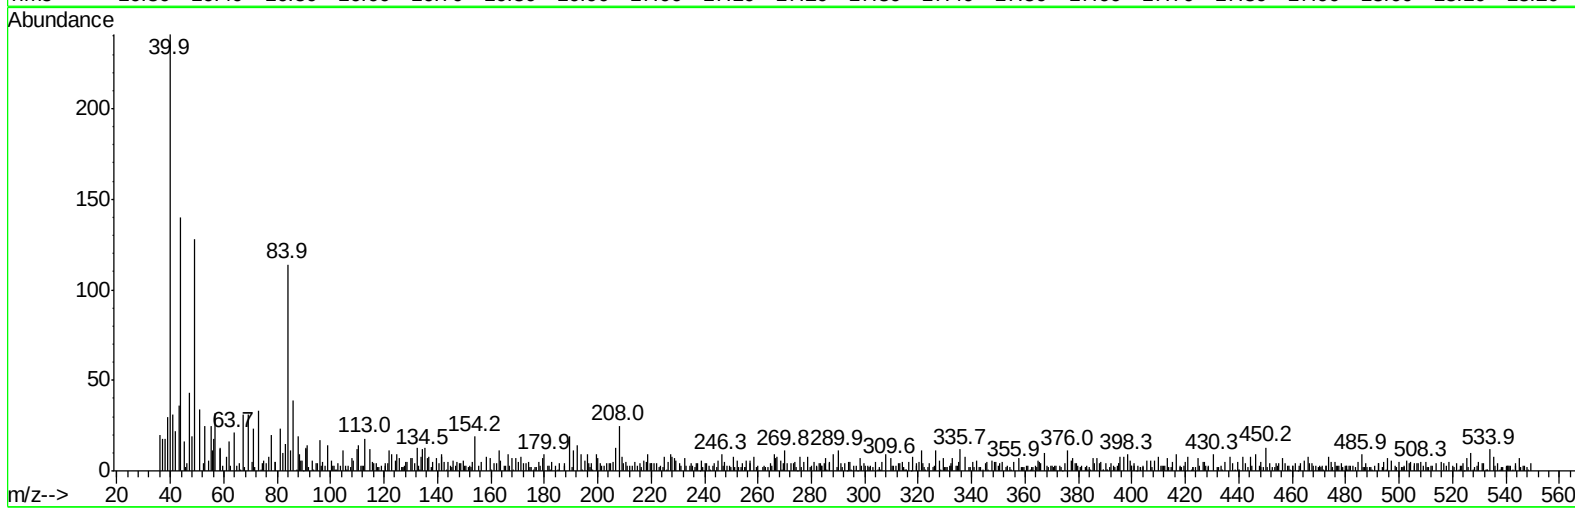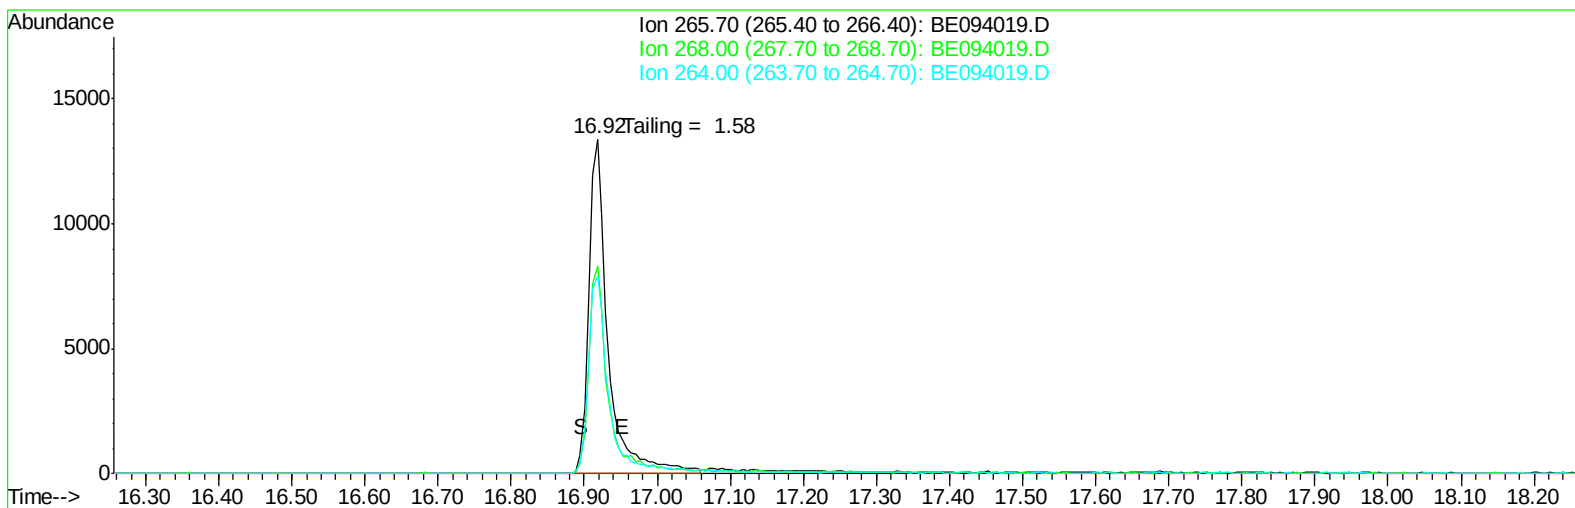

TIC: BE094019.D

(69) Pentachlorophenol (C)

11.219min (+0.250) 185.53ng

response 10

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.67
264.00	64.60	66.67
0.00	0.00	0.00