


Data Path : Z:\HPCHEM1\BNA E\Data\BE091817\
 Data File : BE094019.D
 Acq On : 18 Sep 2017 10:01
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE090517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 13:34:56 2017

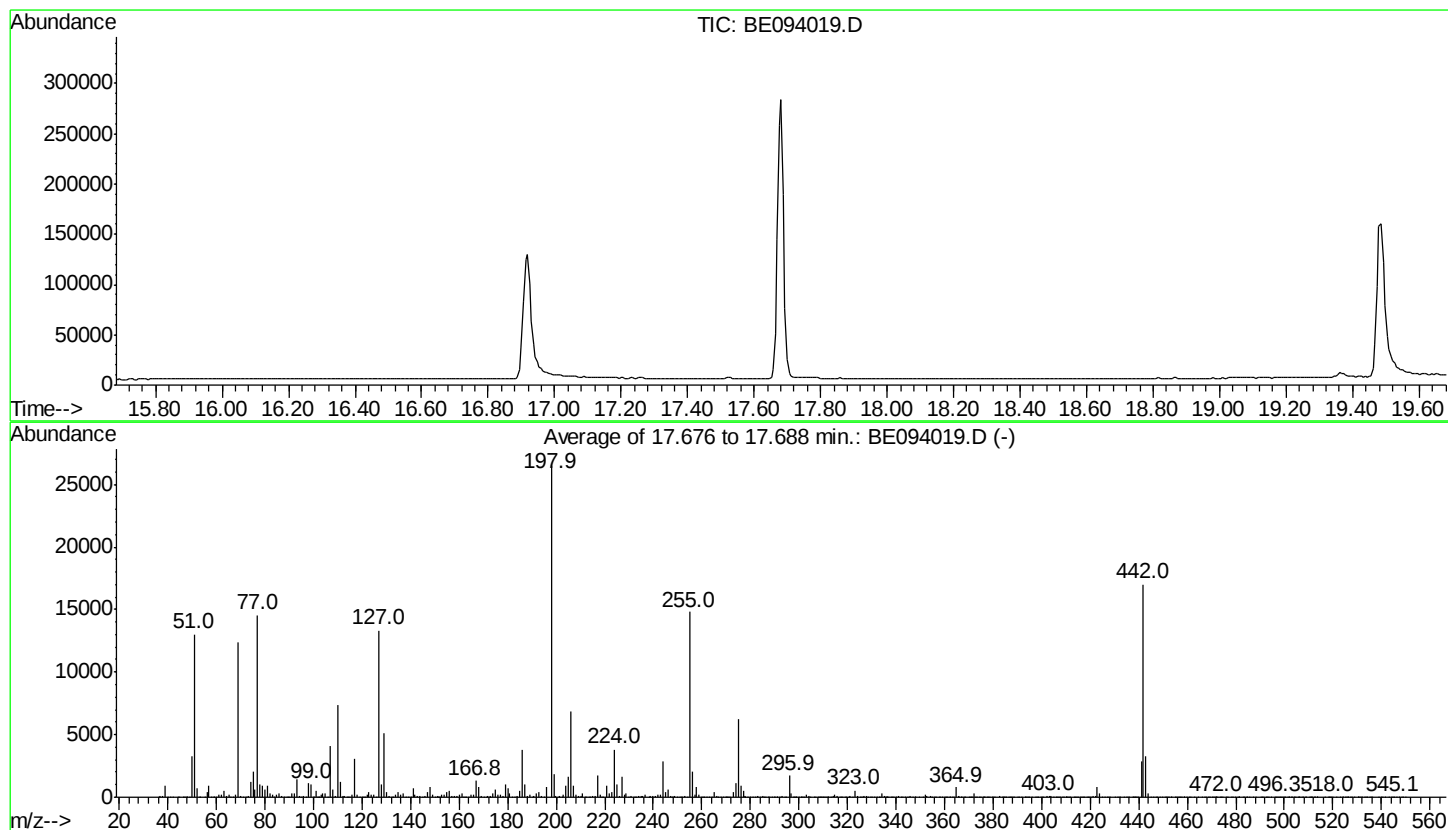

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.2	13041	PASS
68	69	0.00	2	1.4	172	PASS
69	198	0.00	100	46.5	12332	PASS
70	69	0.00	2	0.6	72	PASS
127	198	10	80	50.3	13322	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26498	PASS
199	198	5	9	6.8	1809	PASS
275	198	10	60	23.7	6274	PASS
365	198	1	100	3.0	793	PASS
441	442	0.01	24	17.0	2892	PASS
442	198	50	100	64.1	16988	PASS
443	442	15	24	19.1	3246	PASS