
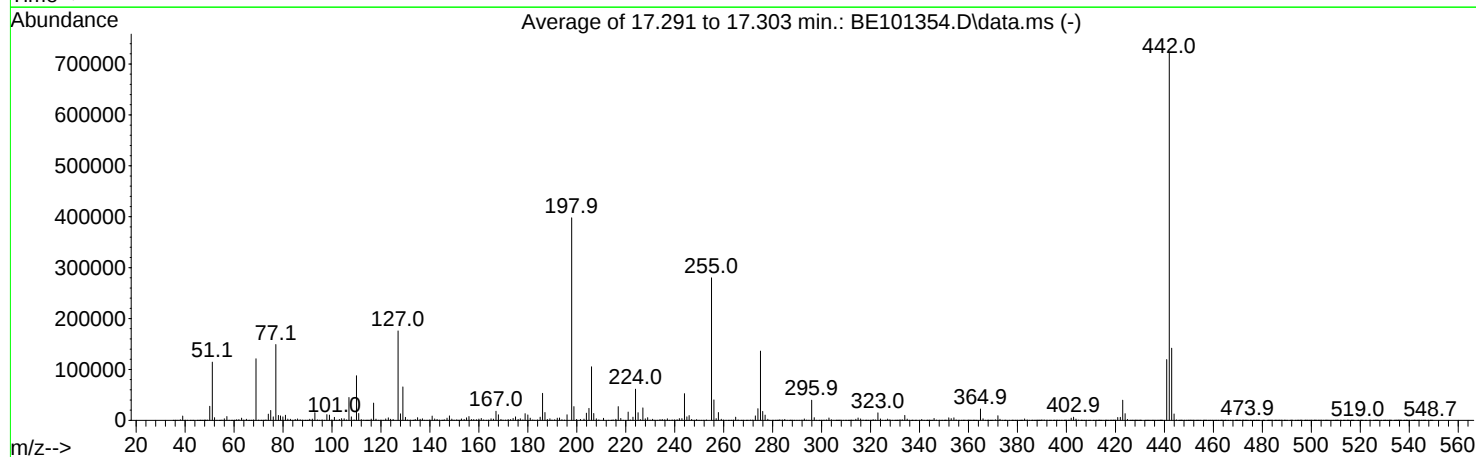


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091824\
Data File : BE101354.D
Acq On : 18 Sep 2024 8:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 17 16:03:42 2024

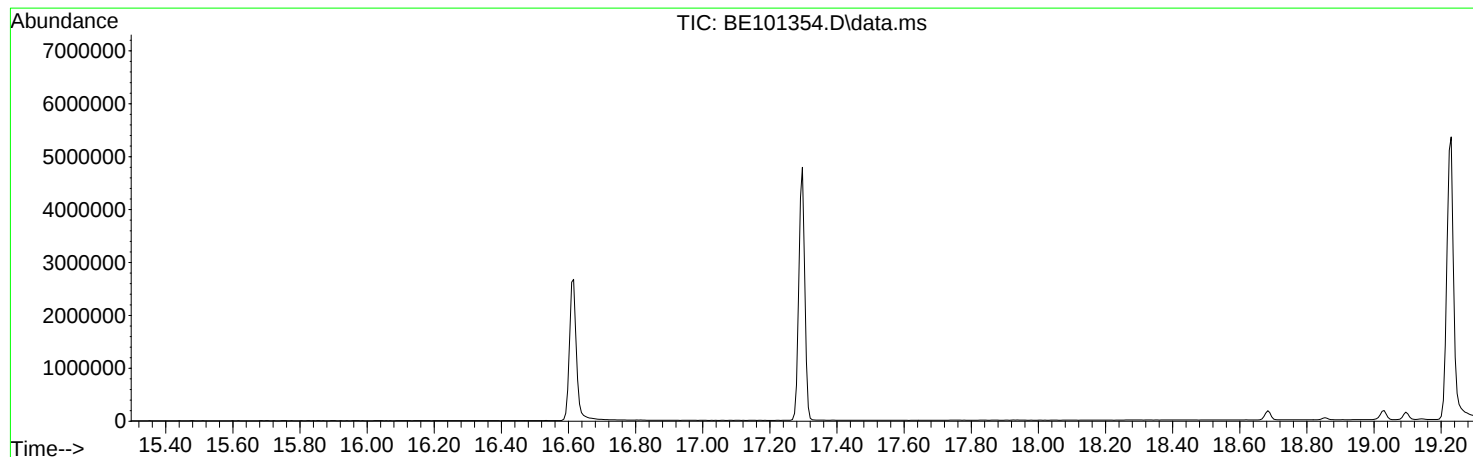




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	114422	PASS
68	69	0.00	2	0.8	923	PASS
69	198	0.00	100	30.4	121021	PASS
70	69	0.00	2	0.5	549	PASS
127	198	10	80	44.1	175696	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	397965	PASS
199	198	5	9	6.8	27035	PASS
275	198	10	60	34.2	135996	PASS
365	198	1	100	5.7	22491	PASS
441	198	0.01	100	30.0	119487	PASS
442	442	50	100	100.0	722603	PASS
443	442	15	24	19.6	141826	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091824\
Data File : BE101354.D
Acq On : 18 Sep 2024 8:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Sep 19 03:14:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 17 16:03:42 2024
Response via : Initial Calibration

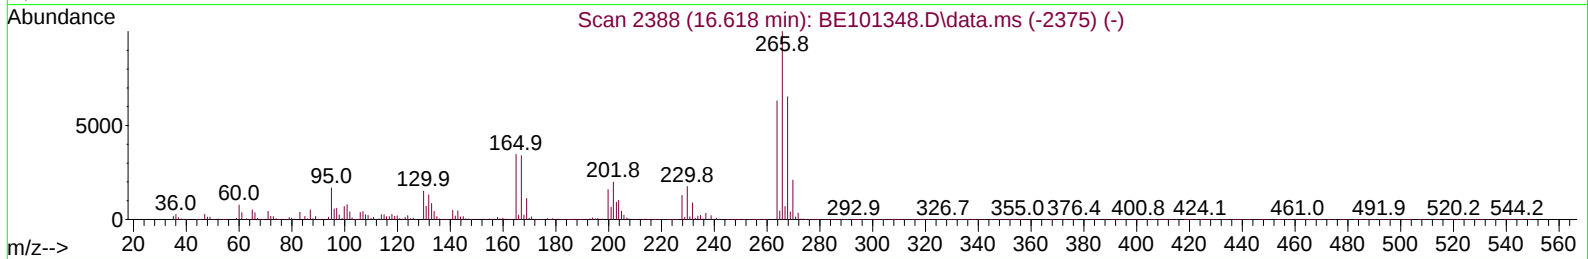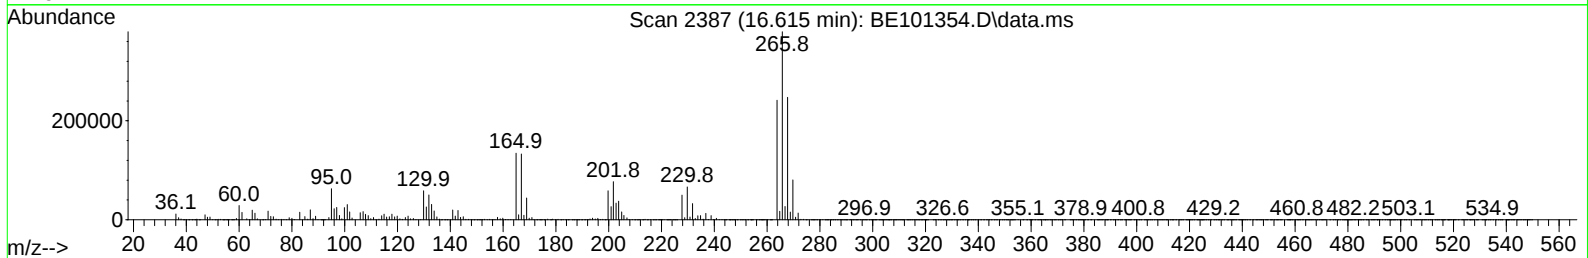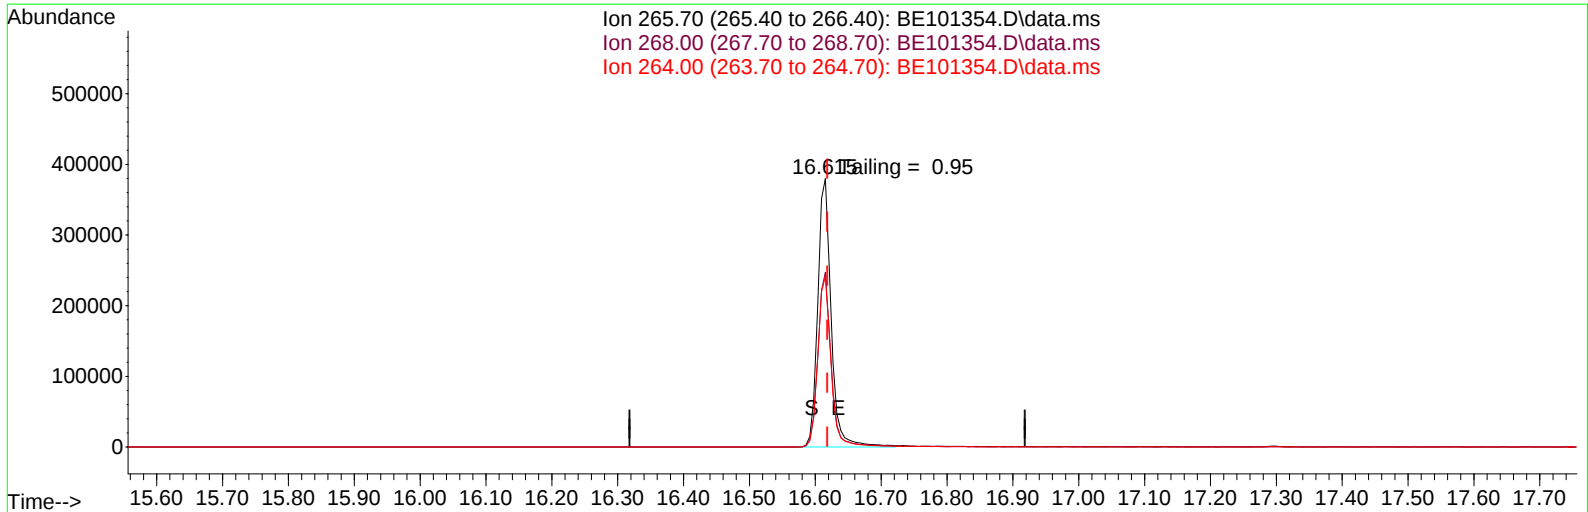

TIC: BE101354.D\data.ms

(70) Pentachlorophenol (C)

16.615min (-0.003) 189932.65 ng




response 542406

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.11
264.00	63.10	63.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091824\
Data File : BE101354.D
Acq On : 18 Sep 2024 8:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Sep 19 03:14:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 17 16:03:42 2024
Response via : Initial Calibration

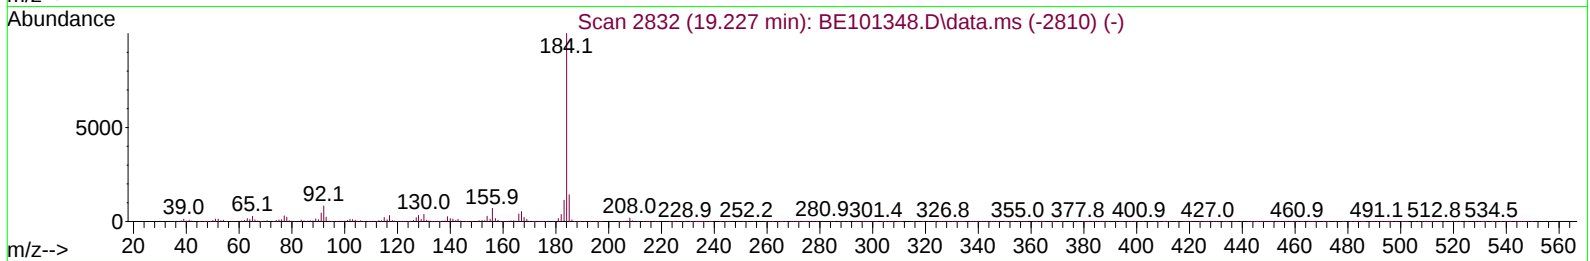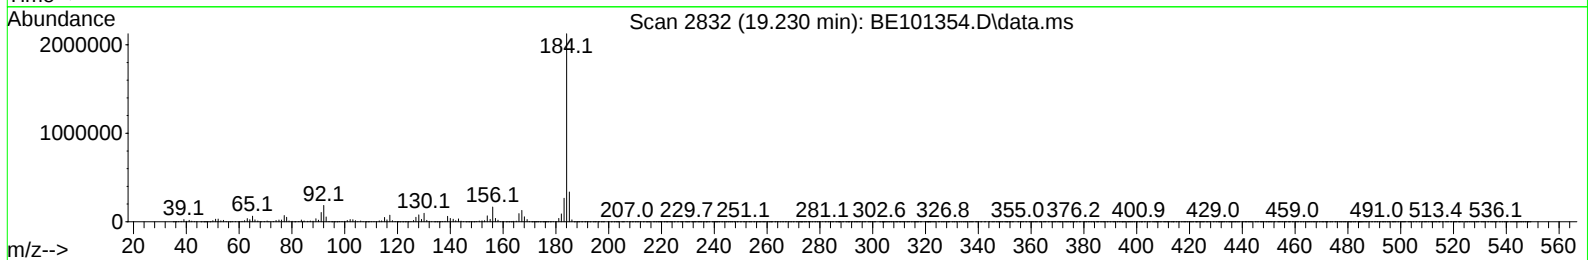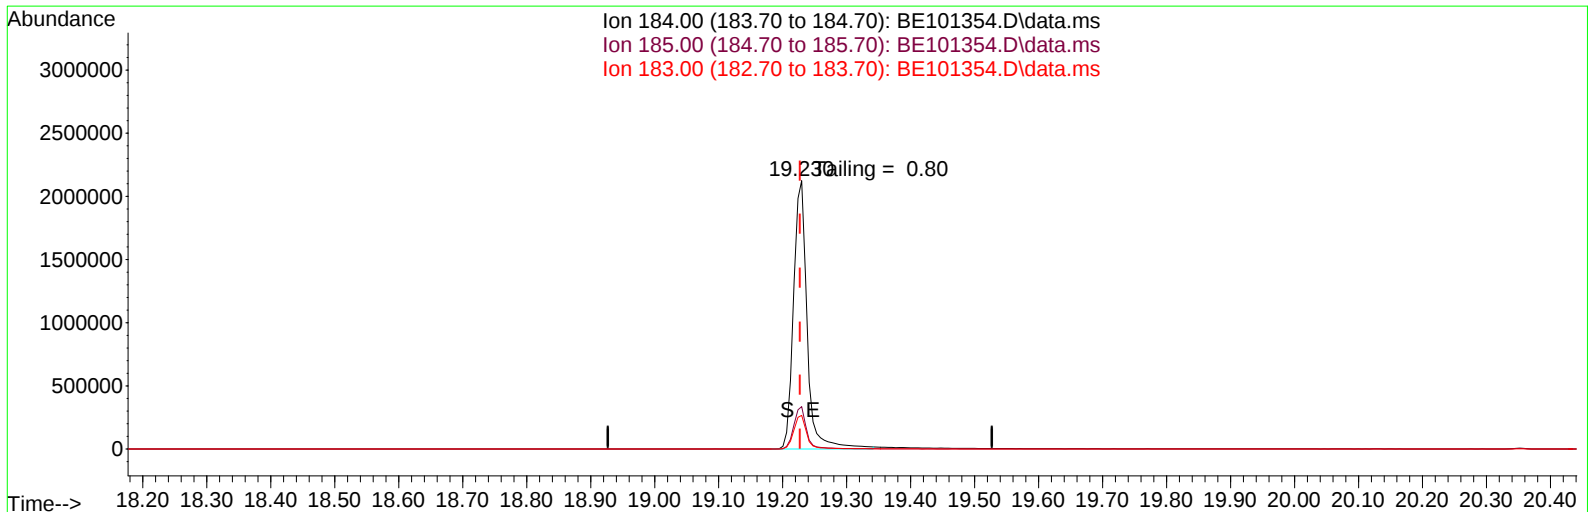

TIC: BE101354.D\data.ms

(77) Benzidine

19.230min (+ 0.003) 183944.78 ng

response 3211613

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	15.83
183.00	11.40	12.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/18/2024	BNA_E	<u>BE101354.D</u>
Compound Name	Response	Retention Time
DDT	1787268	20.352
DDD	24825	19.923
DDE	913	19.406
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25738	1813006	1.42

Instrument :
BNA_E
ClientSampleId :
DFTPP