


1,4-Dioxane

Response Ratio

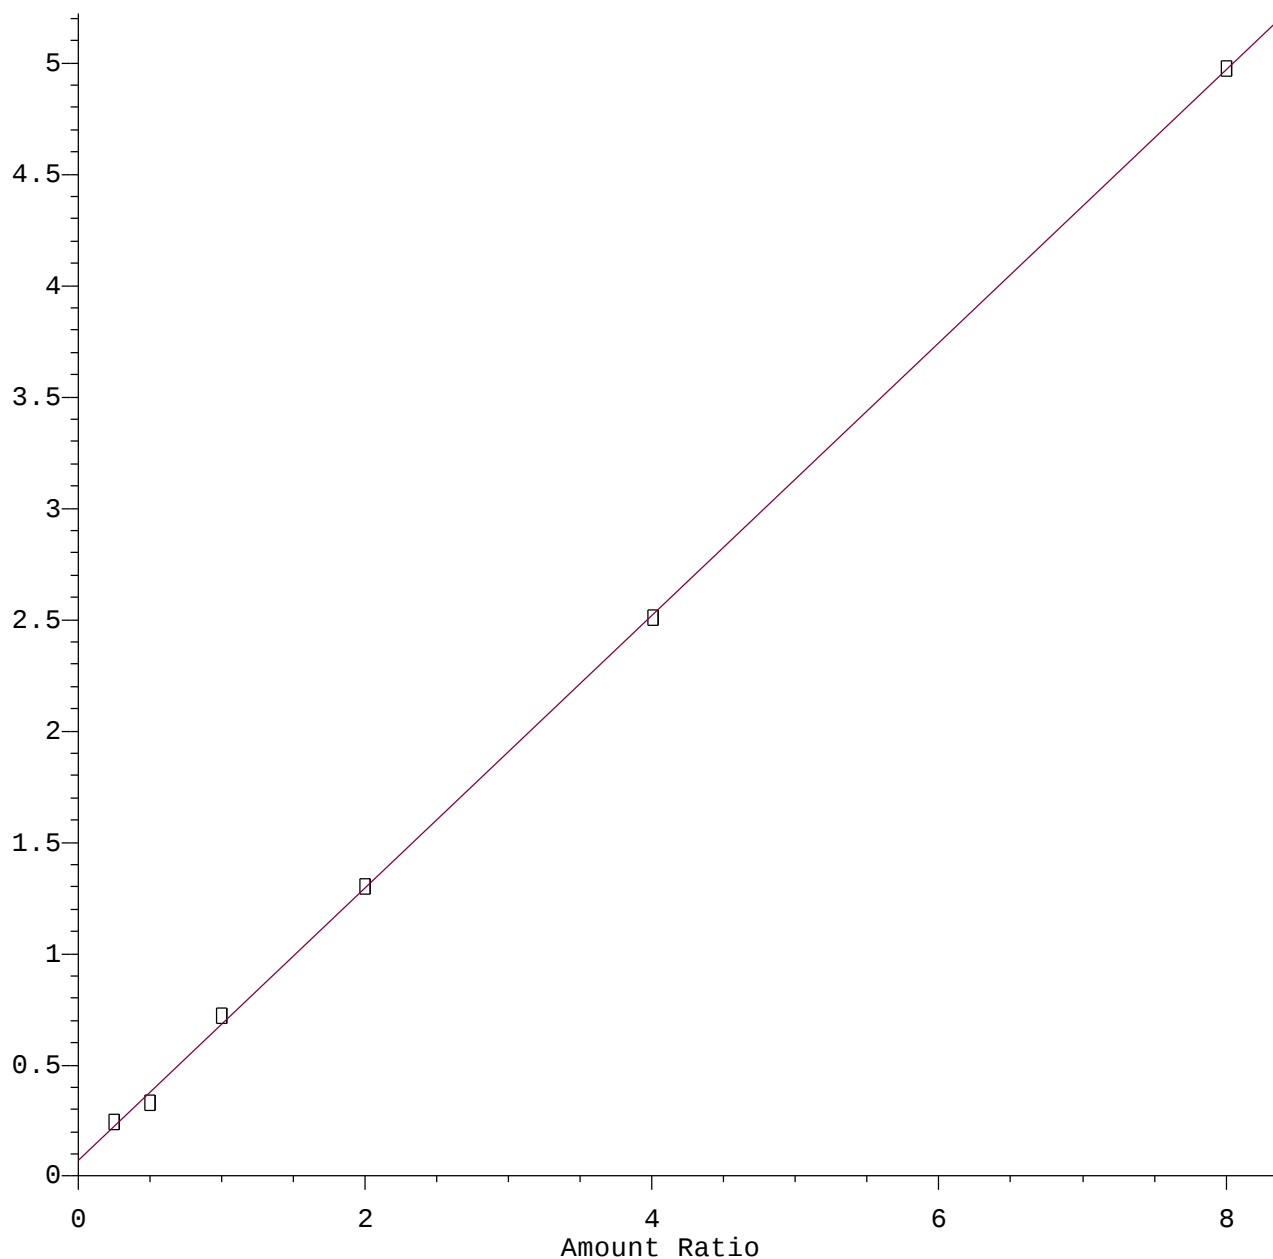


Resp Ratio = $6.12 \times 10^{-1} \times \text{Amt} + 7.08 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091918.M
Calibration Table Last Updated: Thu Sep 20 10:54:43 2018

n-Nitrosodimethylamine

Response Ratio

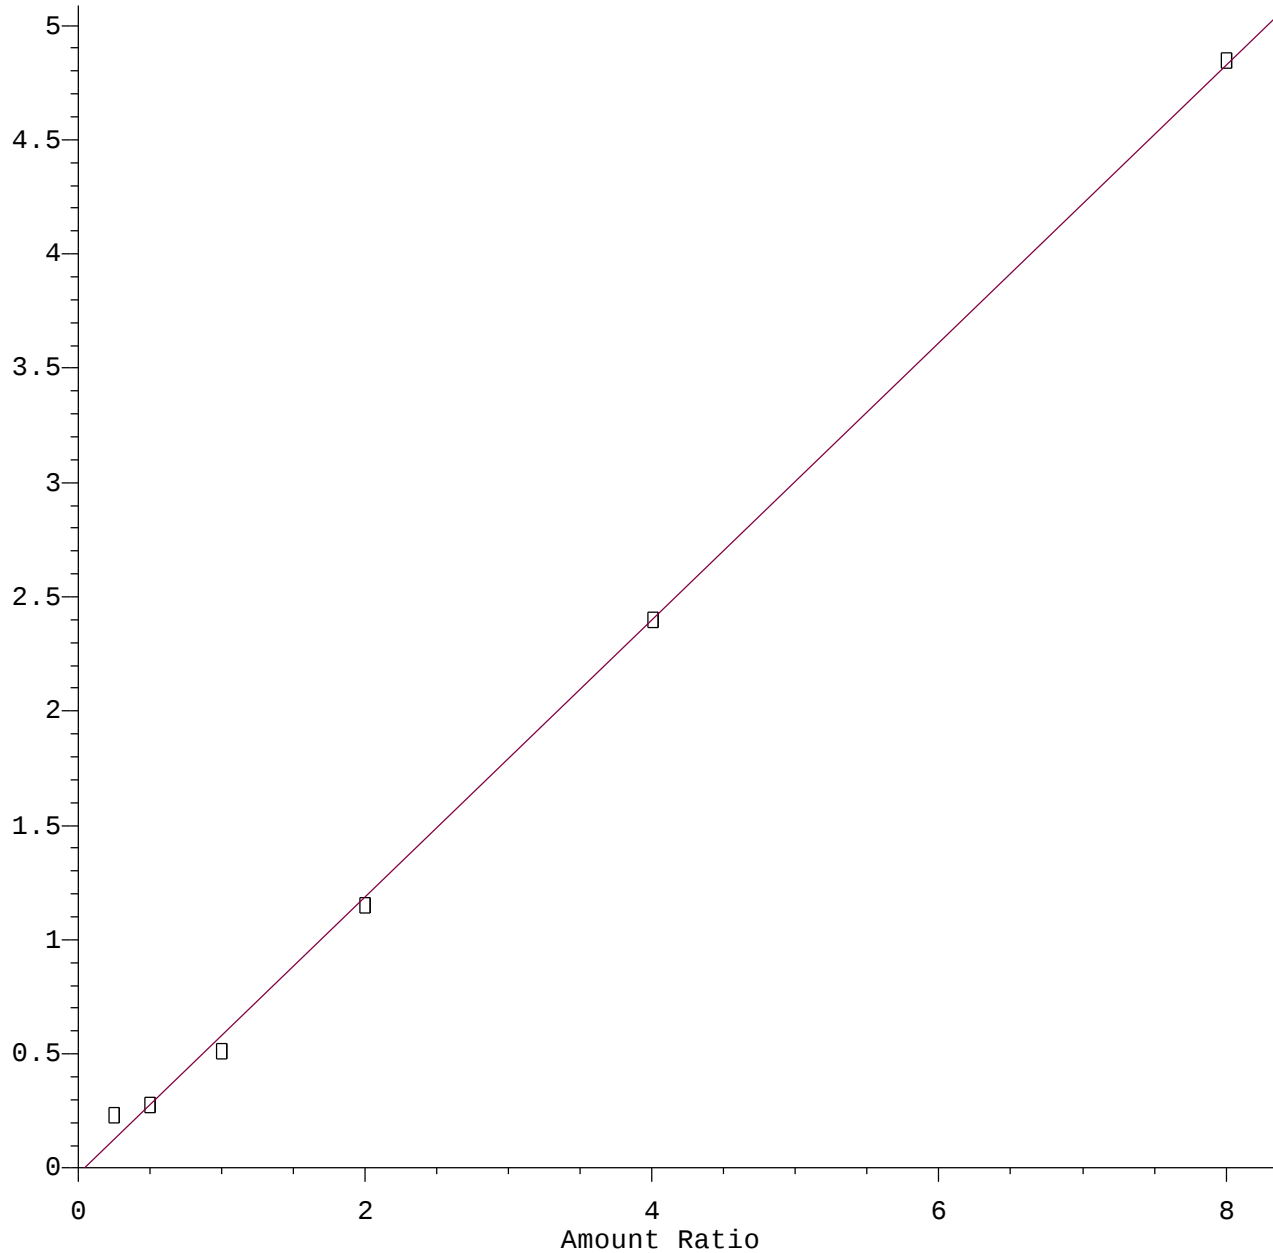


Resp Ratio = $6.06 \times 10^{-1} \times \text{Amt} - 2.50 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091918.M
Calibration Table Last Updated: Thu Sep 20 10:54:43 2018


2,4,6-Tribromophenol

Response Ratio

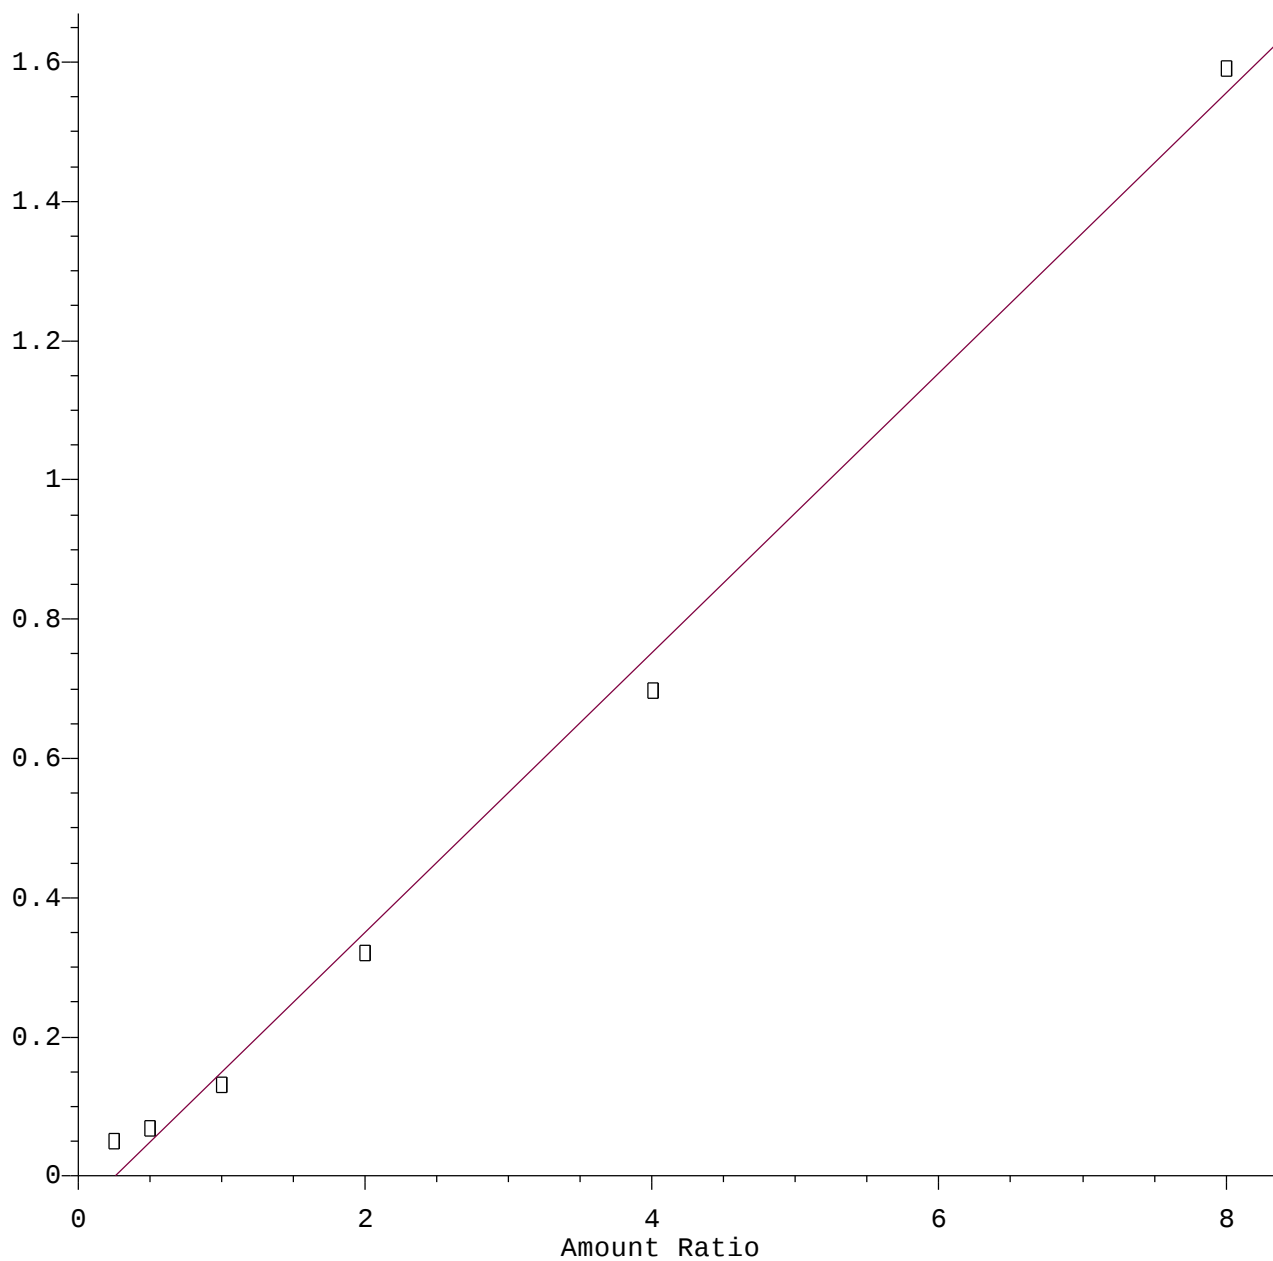

Resp Ratio = $2.01 \times 10^{-1} \times \text{Amt} - 5.15 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091918.M
Calibration Table Last Updated: Thu Sep 20 10:54:43 2018

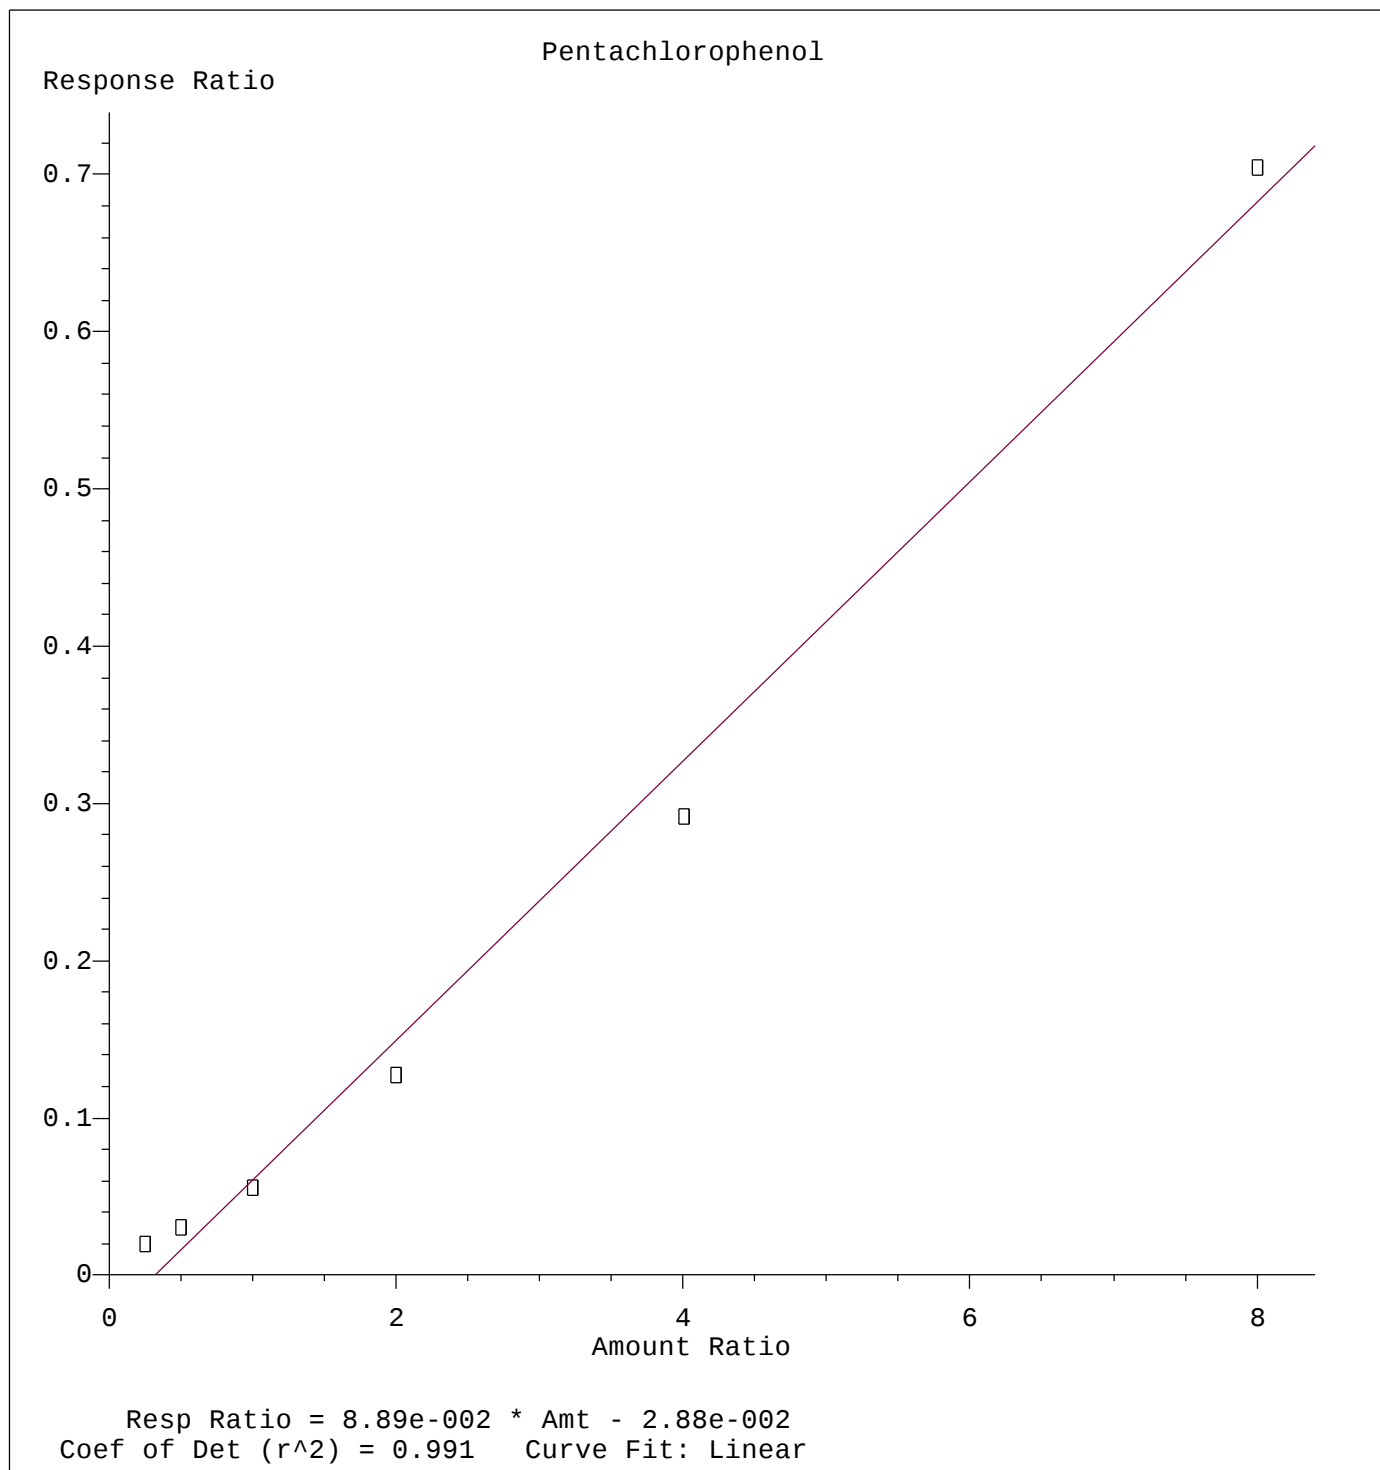

Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091918.M
Calibration Table Last Updated: Thu Sep 20 10:54:43 2018


Bis(2-ethylhexyl)phthalate

Response Ratio

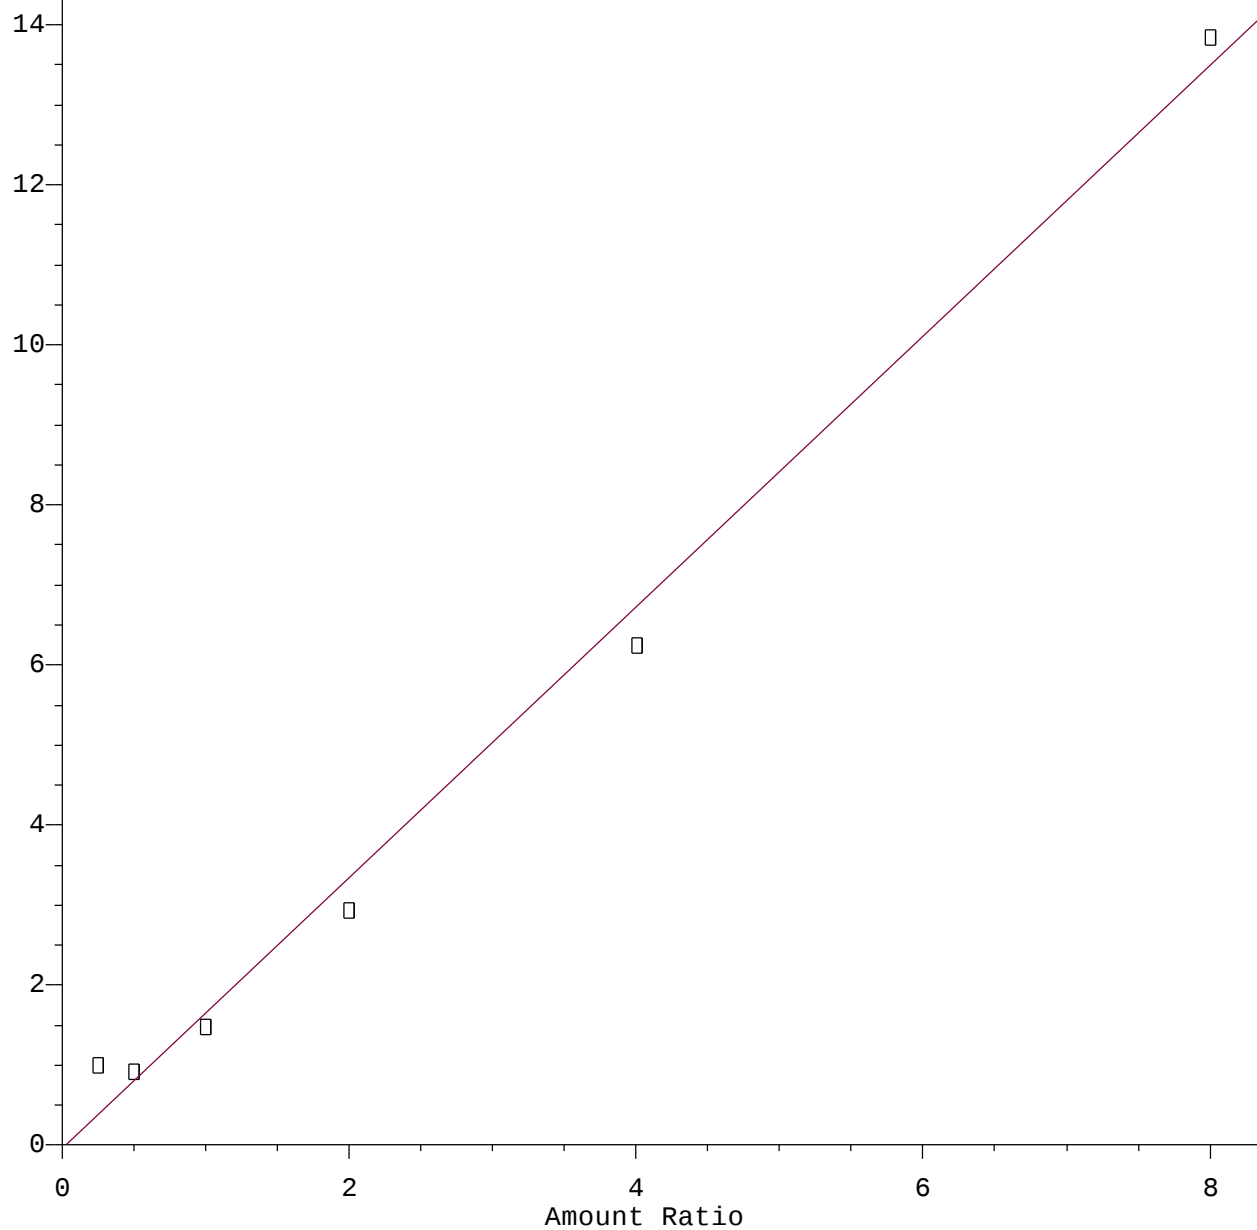

Resp Ratio = 1.69e+000 * Amt - 4.43e-002
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091918.M
Calibration Table Last Updated: Thu Sep 20 10:54:43 2018

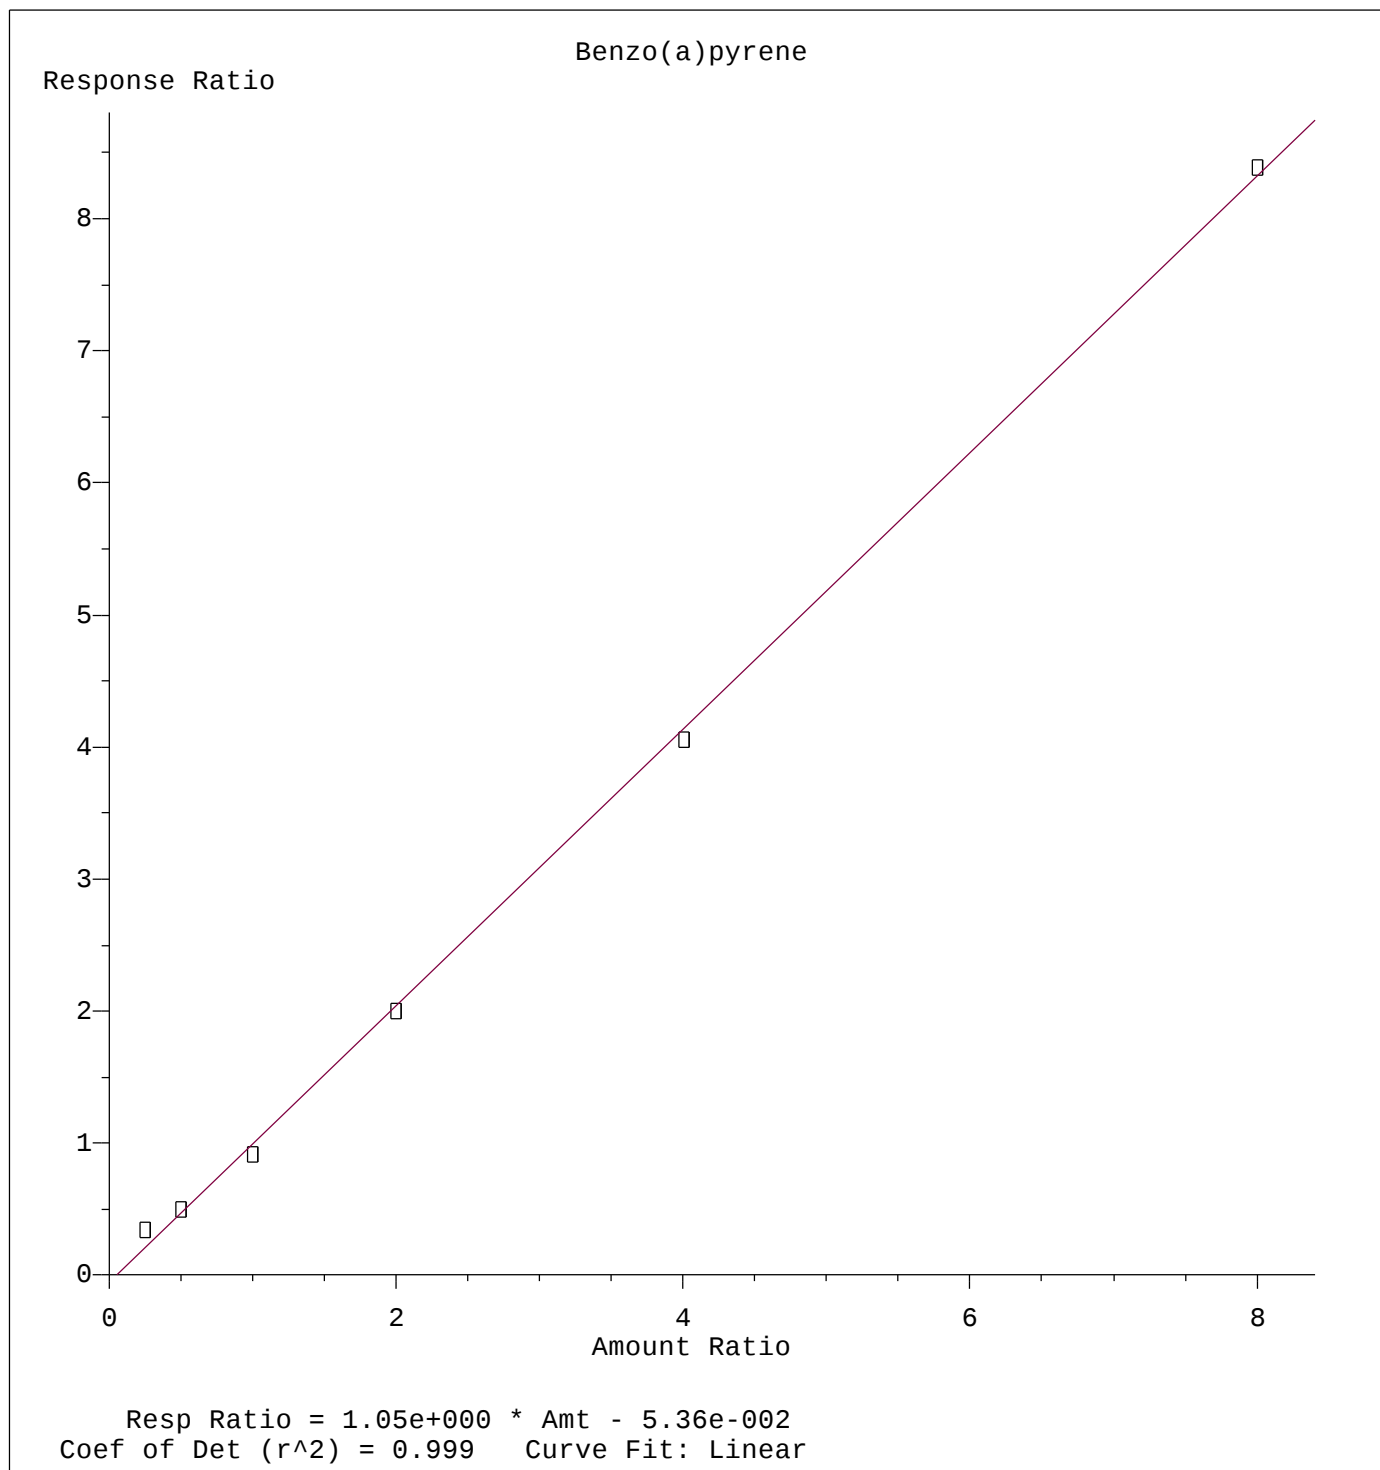

Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091918.M
Calibration Table Last Updated: Thu Sep 20 10:54:43 2018