
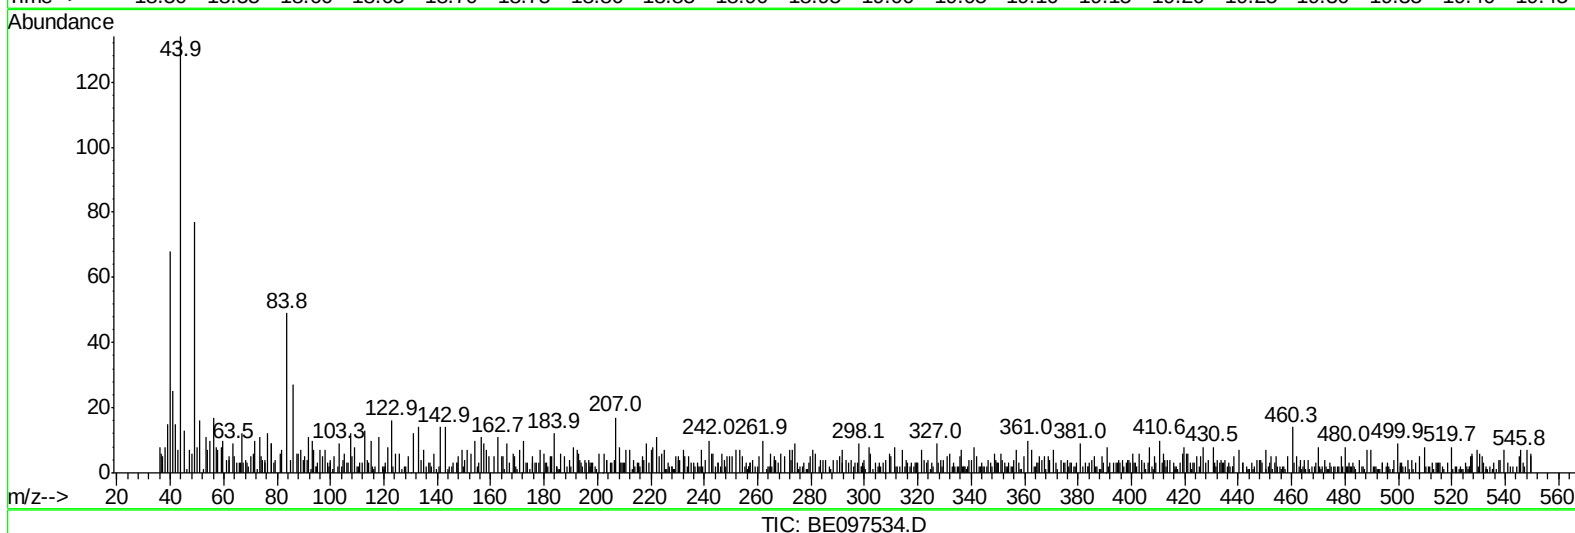


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091918\
Data File : BE097534.D
Acq On : 19 Sep 2018 11:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 08:16:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 14 13:26:52 2018
Response via : Initial Calibration

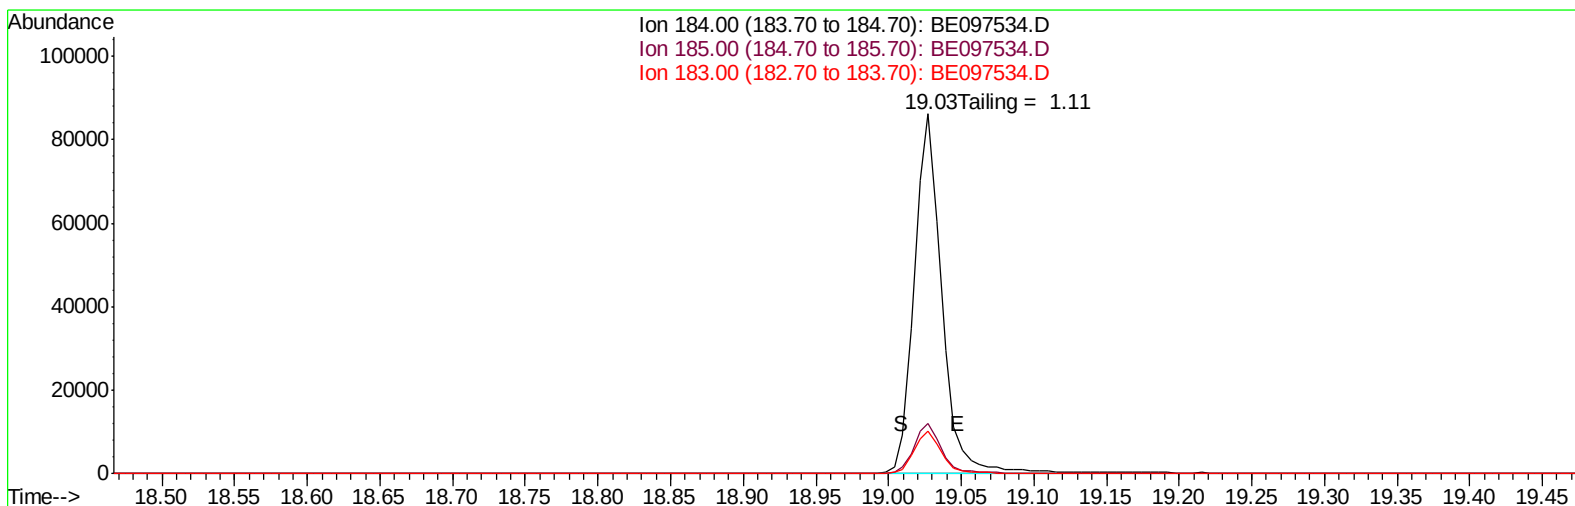

(76) Benzidine



12.711min (+0.158) 23.54ng

response 5

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	42.86#
183.00	11.60	35.71#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091918\
Data File : BE097534.D
Acq On : 19 Sep 2018 11:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 08:16:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 14 13:26:52 2018
Response via : Initial Calibration

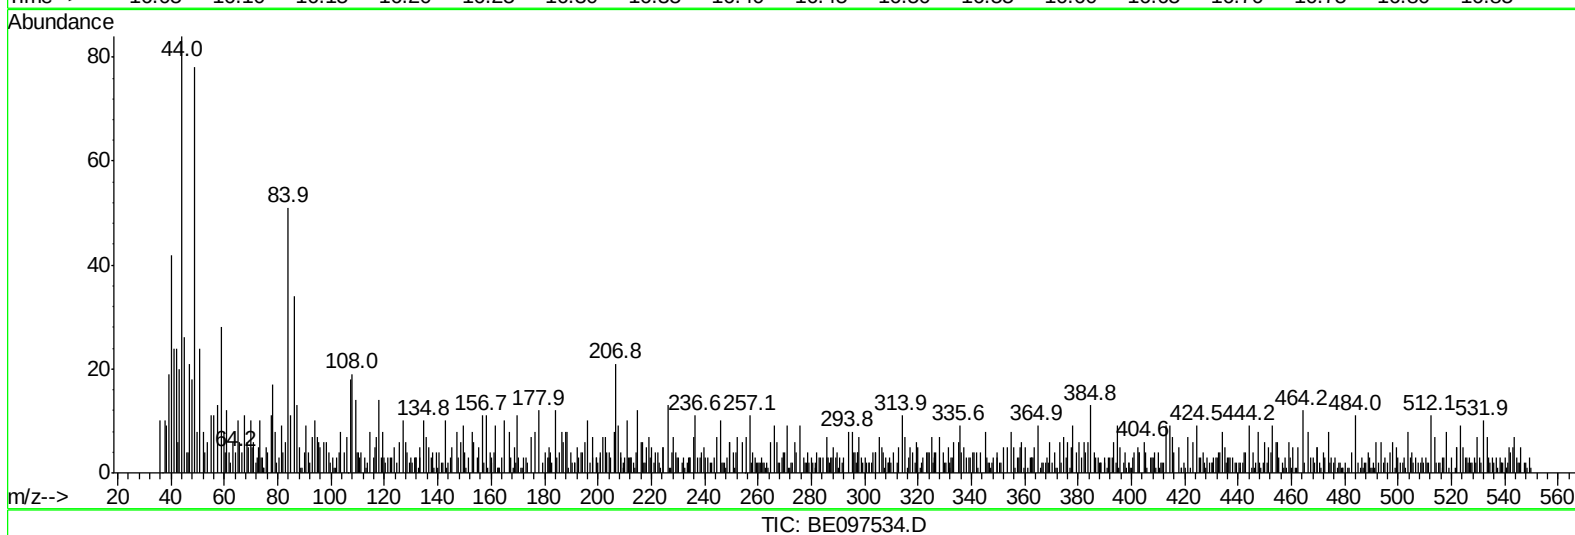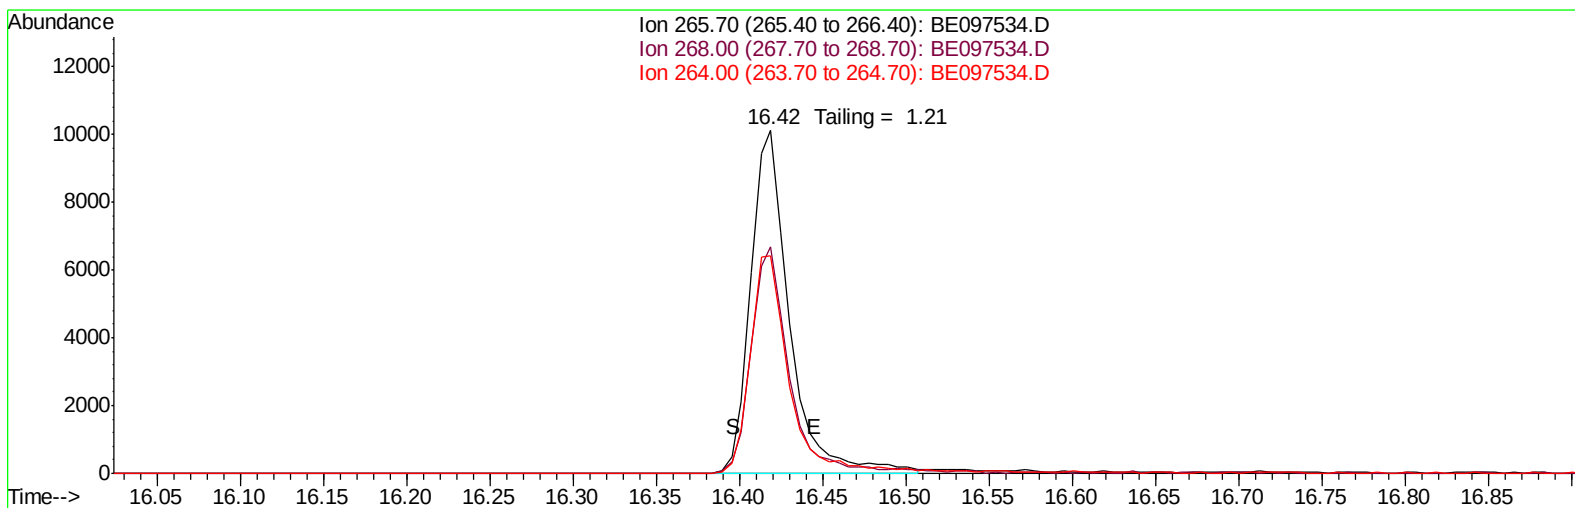

TIC: BE097534.D

(69) Pentachlorophenol (C)

11.066min (+0.024) 81.01ng

response 5

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	44.44#
264.00	61.90	77.78#
0.00	0.00	0.00