
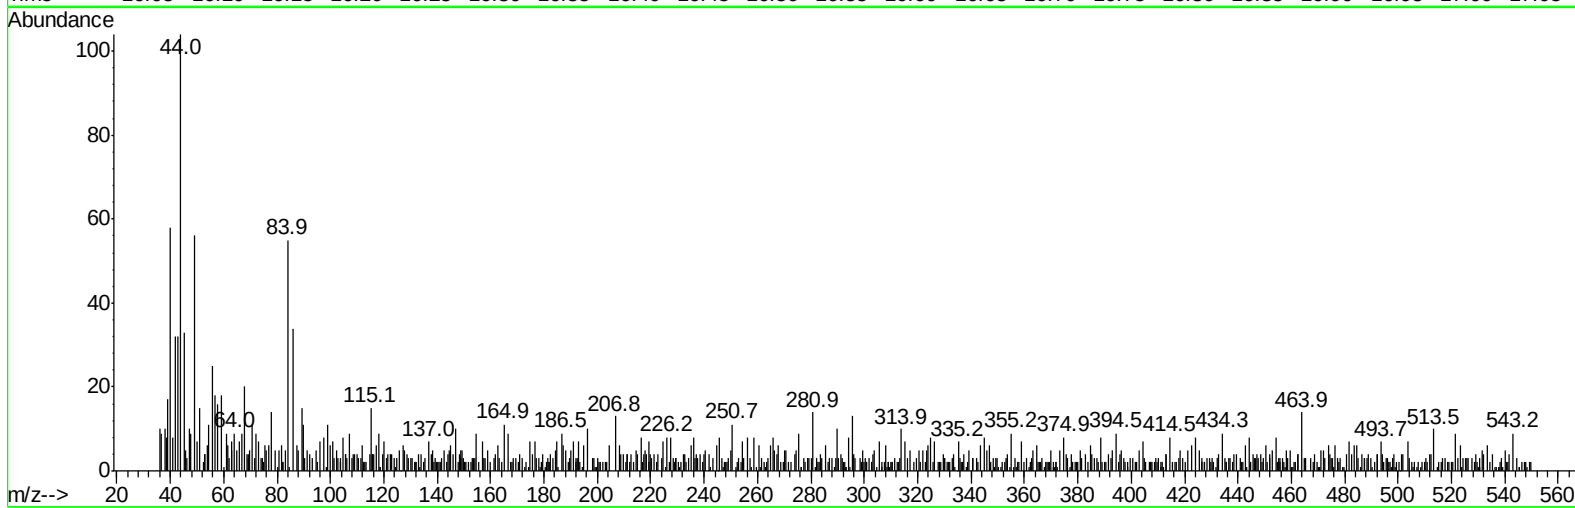


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091918\
Data File : BE097543.D
Acq On : 19 Sep 2018 16:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 08:17:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 14 13:26:52 2018
Response via : Initial Calibration

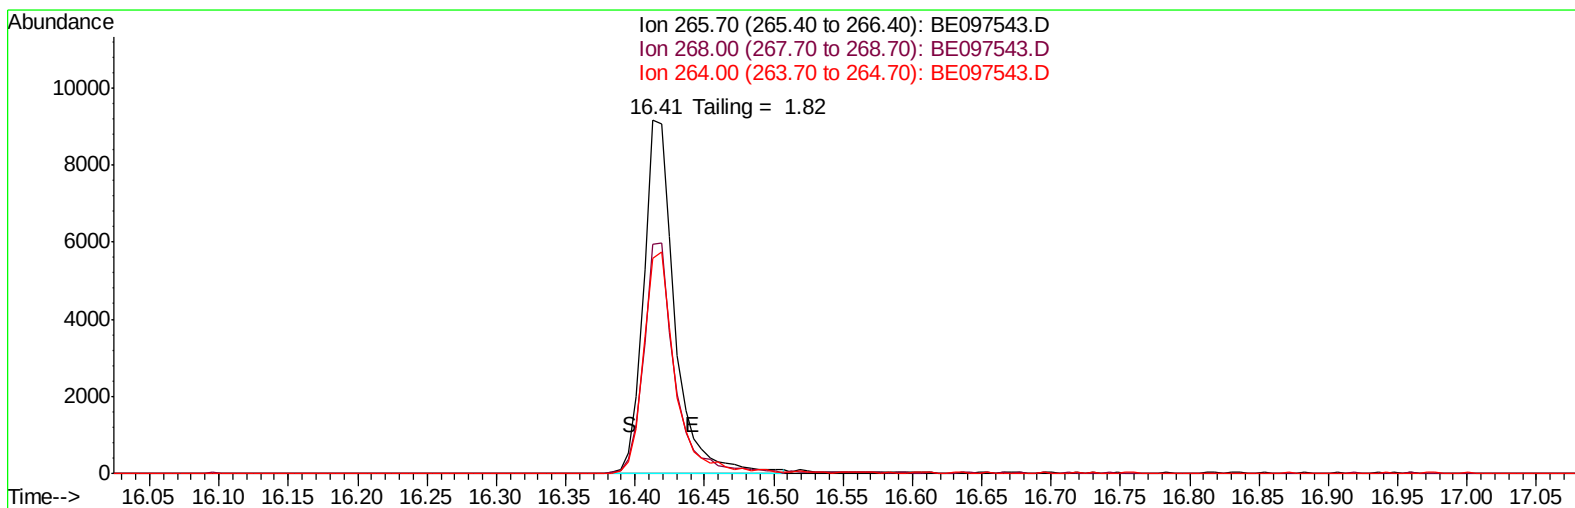

TIC: BE097543.D

(69) Pentachlorophenol (C)



10.849min (-0.193) 32.40ng

response 2

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.54
264.00	61.90	69.23
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE091918\
Data File : BE097543.D
Acq On : 19 Sep 2018 16:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 08:17:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 14 13:26:52 2018
Response via : Initial Calibration

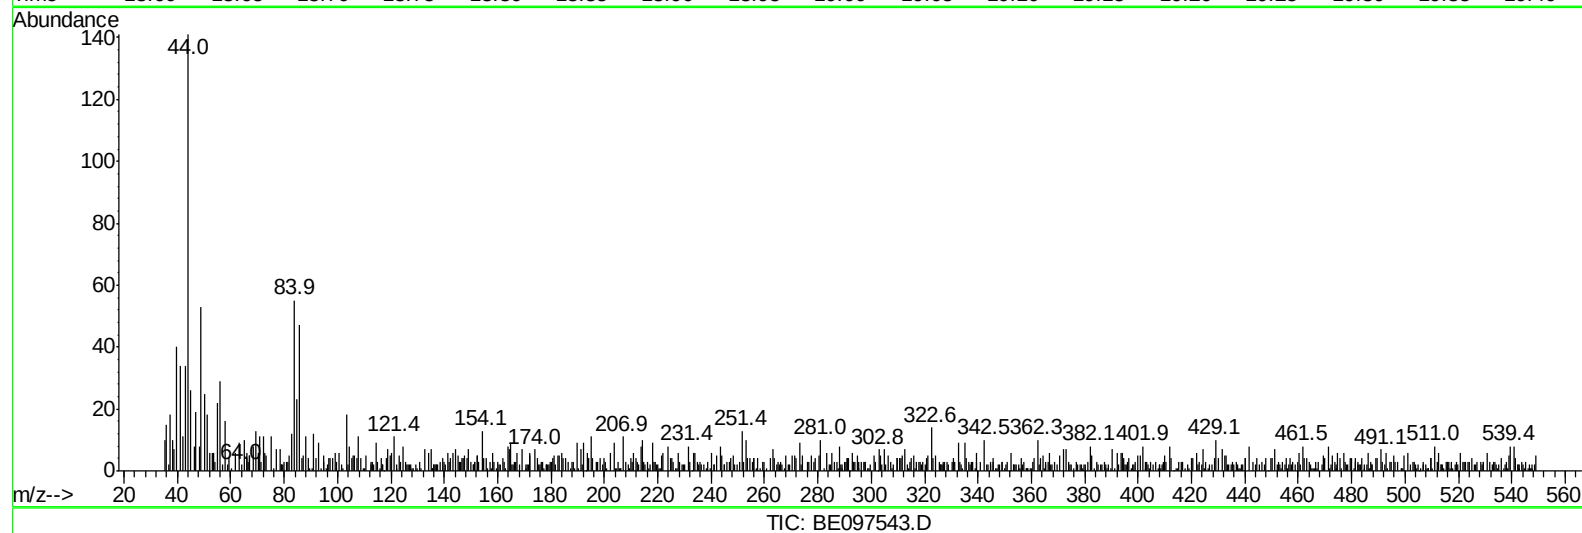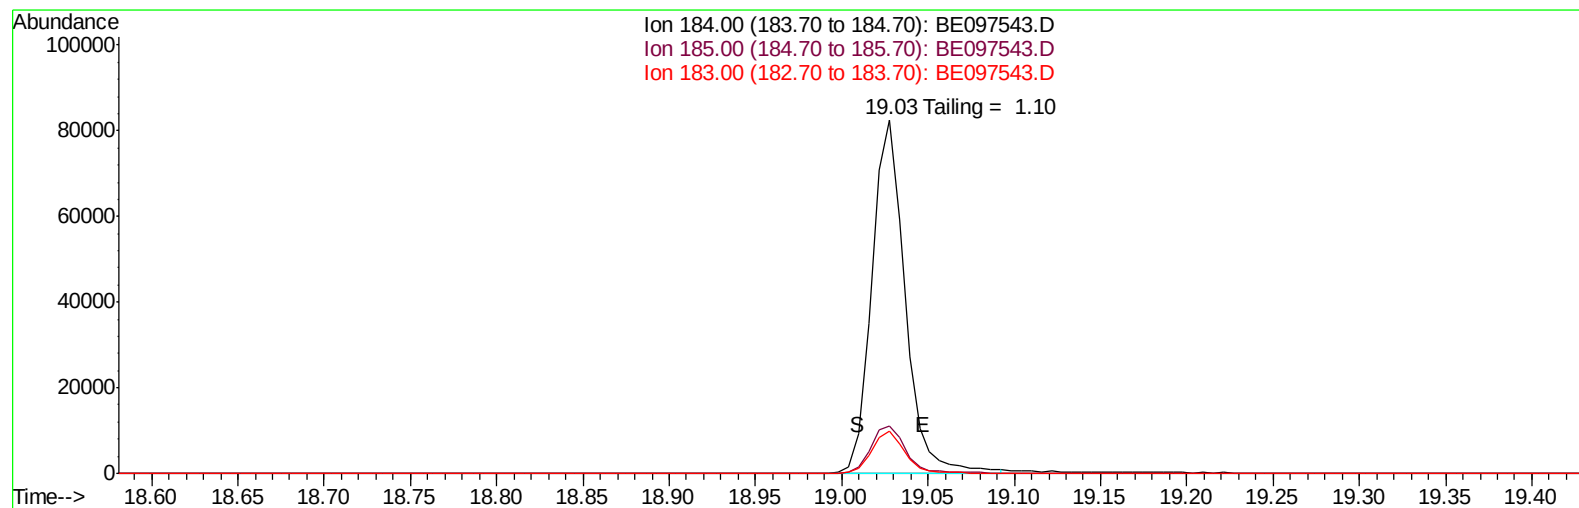

(76) Benzidine

12.535min (-0.018) 2.82ng

response 1

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	80.00#
183.00	11.60	50.00#
0.00	0.00	0.00