


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE091918\
 Data File : BE097534.D
 Acq On : 19 Sep 2018 11:01
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 20 10:54:43 2018

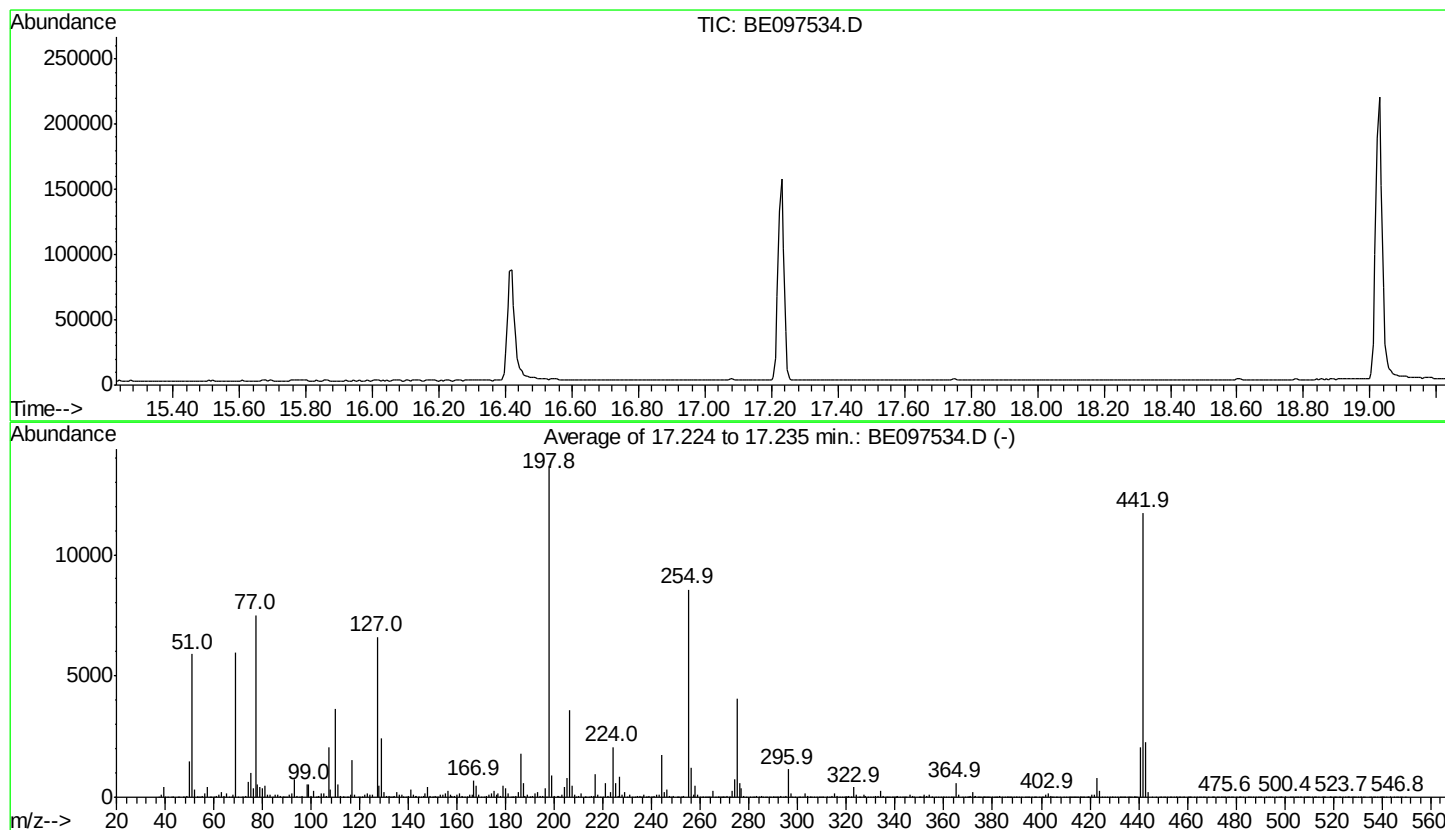

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	5890	PASS
68	69	0.00	2	1.9	111	PASS
69	198	0.00	100	43.5	5940	PASS
70	69	0.00	2	0.3	18	PASS
127	198	10	80	48.4	6610	PASS
197	198	0.00	2	0.1	20	PASS
198	198	100	100	100.0	13670	PASS
199	198	5	9	6.4	876	PASS
275	198	10	60	29.7	4064	PASS
365	198	1	100	4.3	581	PASS
441	198	0.01	100	14.9	2037	PASS
442	198	50	100	85.8	11726	PASS
443	442	15	24	19.2	2247	PASS