


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE091918\
Data File : BE097543.D
Acq On : 19 Sep 2018 16:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE091918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 20 10:54:43 2018

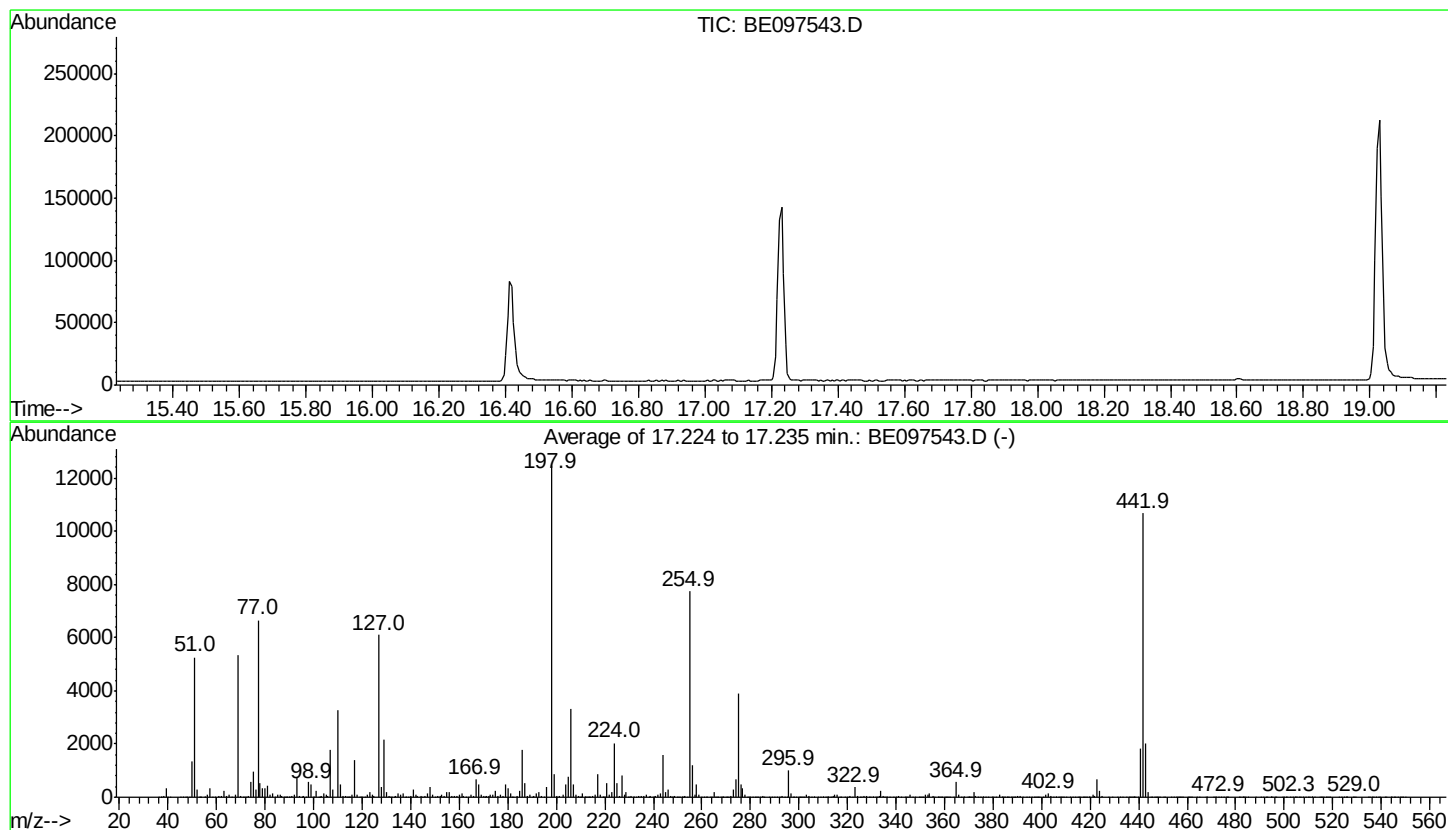

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	5256	PASS
68	69	0.00	2	1.8	95	PASS
69	198	0.00	100	42.9	5353	PASS
70	69	0.00	2	0.6	32	PASS
127	198	10	80	48.9	6101	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12470	PASS
199	198	5	9	6.8	852	PASS
275	198	10	60	31.1	3884	PASS
365	198	1	100	4.5	557	PASS
441	198	0.01	100	14.9	1854	PASS
442	198	50	100	85.6	10676	PASS
443	442	15	24	18.8	2007	PASS