

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091924\
 Data File : BE101371.D
 Acq On : 19 Sep 2024 9:53
 Operator : RC/JU
 Sample : PB163138BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB163138BL

Quant Time: Sep 19 11:10:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 17 16:03:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.576	152	128515	20.000	ng	0.00
21) Naphthalene-d8	10.344	136	554225	20.000	ng	0.00
39) Acenaphthene-d10	14.180	164	372044	20.000	ng	0.00
64) Phenanthrene-d10	16.918	188	938865	20.000	ng	0.00
76) Chrysene-d12	21.078	240	1194399	20.000	ng	0.00
86) Perylene-d12	23.369	264	1598192	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.326	112	1001194	136.212	ng	0.00
7) Phenol-d6	6.953	99	1274619	122.326	ng	0.00
23) Nitrobenzene-d5	8.787	82	722633	82.662	ng	0.00
42) 2,4,6-Tribromophenol	15.690	330	788310	125.976	ng	0.00
45) 2-Fluorobiphenyl	12.805	172	1881968	87.413	ng	0.00
79) Terphenyl-d14	19.515	244	4081450	75.770	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091924\
Data File : BE101371.D
Acq On : 19 Sep 2024 9:53
Operator : RC/JU
Sample : PB163138BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB163138BL

Quant Time: Sep 19 11:10:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 17 16:03:42 2024
Response via : Initial Calibration

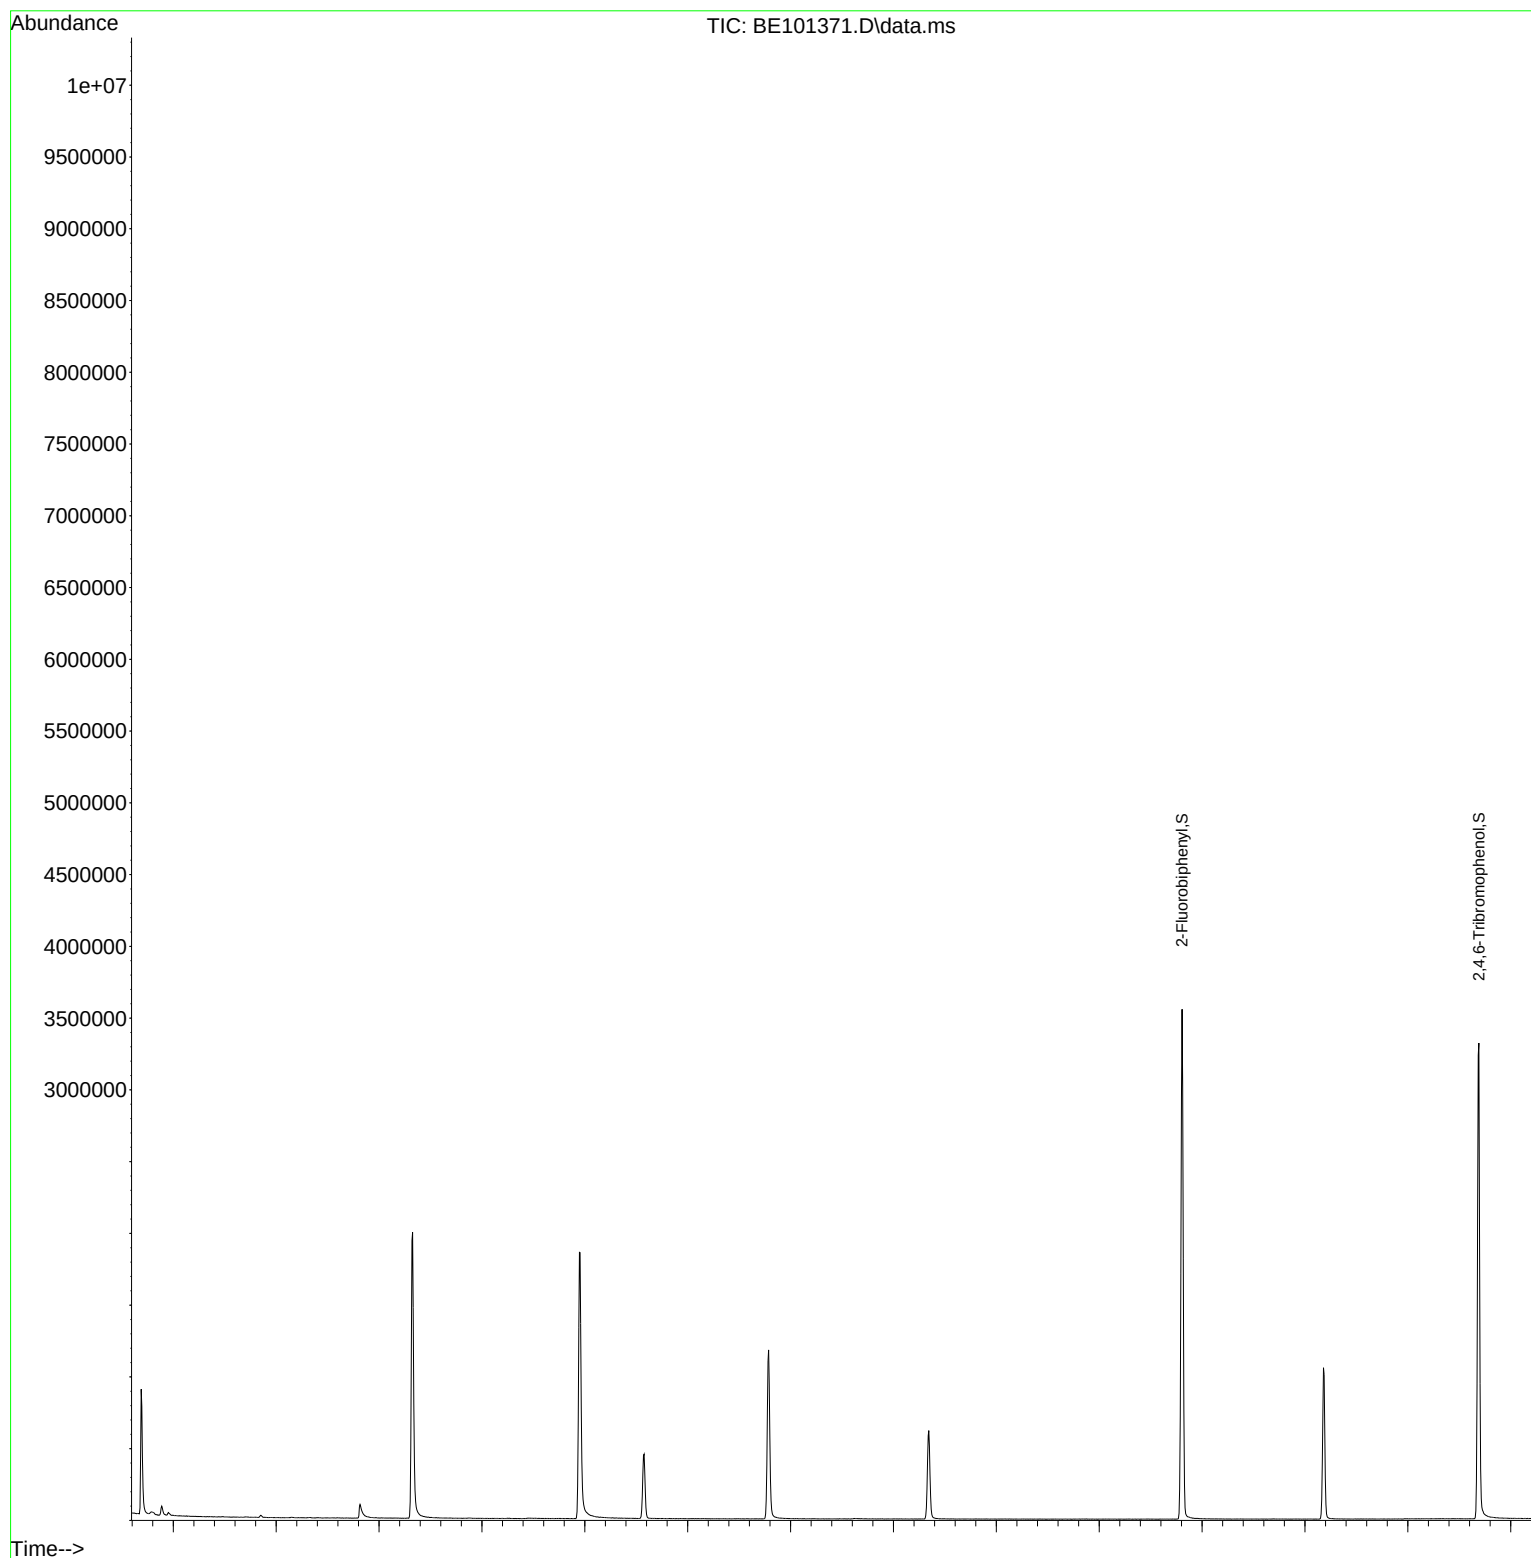

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091924\
Data File : BE101371.D
Acq On : 19 Sep 2024 9:53
Operator : RC/JU
Sample : PB163138BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB163138BL

Quant Time: Sep 19 11:10:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 17 16:03:42 2024
Response via : Initial Calibration

