

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE091924\  
 Data File : BE101376.D  
 Acq On : 19 Sep 2024 13:16  
 Operator : RC/JU  
 Sample : PB163139BL  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 PB163139BL

Quant Time: Sep 19 13:51:54 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE091724.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Sep 17 16:03:42 2024  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc    | Units | Dev(Min) |
|-----------------------------|--------|------|----------|---------|-------|----------|
| -----                       |        |      |          |         |       |          |
| Internal Standards          |        |      |          |         |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.570  | 152  | 128093   | 20.000  | ng    | 0.00     |
| 21) Naphthalene-d8          | 10.344 | 136  | 533234   | 20.000  | ng    | 0.00     |
| 39) Acenaphthene-d10        | 14.180 | 164  | 336195   | 20.000  | ng    | 0.00     |
| 64) Phenanthrene-d10        | 16.918 | 188  | 812706   | 20.000  | ng    | 0.00     |
| 76) Chrysene-d12            | 21.078 | 240  | 1139442  | 20.000  | ng    | 0.00     |
| 86) Perylene-d12            | 23.370 | 264  | 1532871  | 20.000  | ng    | 0.00     |
| System Monitoring Compounds |        |      |          |         |       |          |
| 5) 2-Fluorophenol           | 5.320  | 112  | 985096   | 134.464 | ng    | 0.00     |
| 7) Phenol-d6                | 6.948  | 99   | 1234393  | 118.856 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 8.787  | 82   | 703092   | 83.593  | ng    | 0.00     |
| 42) 2,4,6-Tribromophenol    | 15.690 | 330  | 670737   | 118.616 | ng    | 0.00     |
| 45) 2-Fluorobiphenyl        | 12.806 | 172  | 1757899  | 90.357  | ng    | 0.00     |
| 79) Terphenyl-d14           | 19.515 | 244  | 3797189  | 73.892  | ng    | 0.00     |

Target Compounds Qvalue


-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE091924\  
Data File : BE101376.D  
Acq On : 19 Sep 2024 13:16  
Operator : RC/JU  
Sample : PB163139BL  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
PB163139BL

Quant Time: Sep 19 13:51:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE091724.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 17 16:03:42 2024  
Response via : Initial Calibration

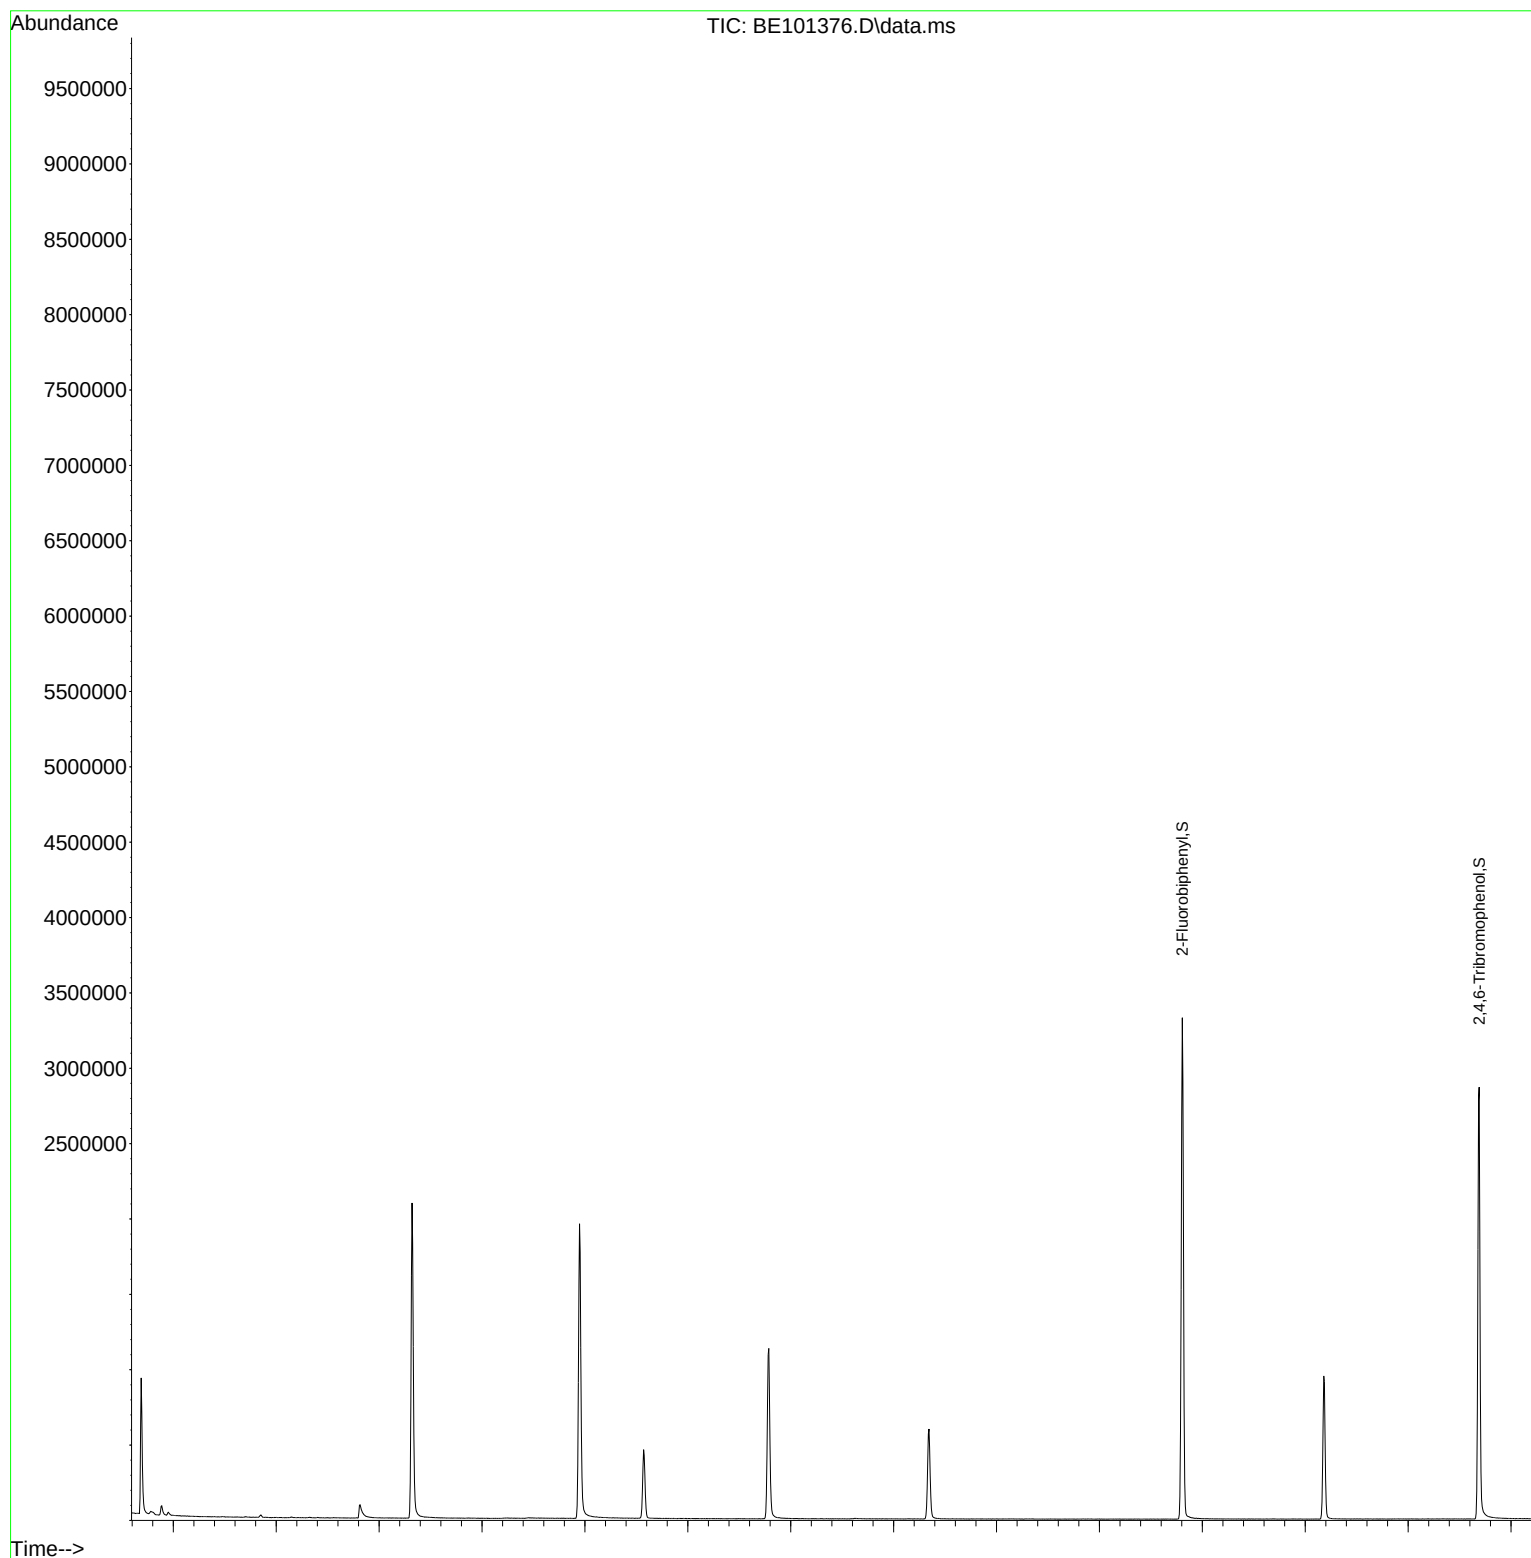

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE091924\  
Data File : BE101376.D  
Acq On : 19 Sep 2024 13:16  
Operator : RC/JU  
Sample : PB163139BL  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
PB163139BL

Quant Time: Sep 19 13:51:54 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE091724.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 17 16:03:42 2024  
Response via : Initial Calibration

