
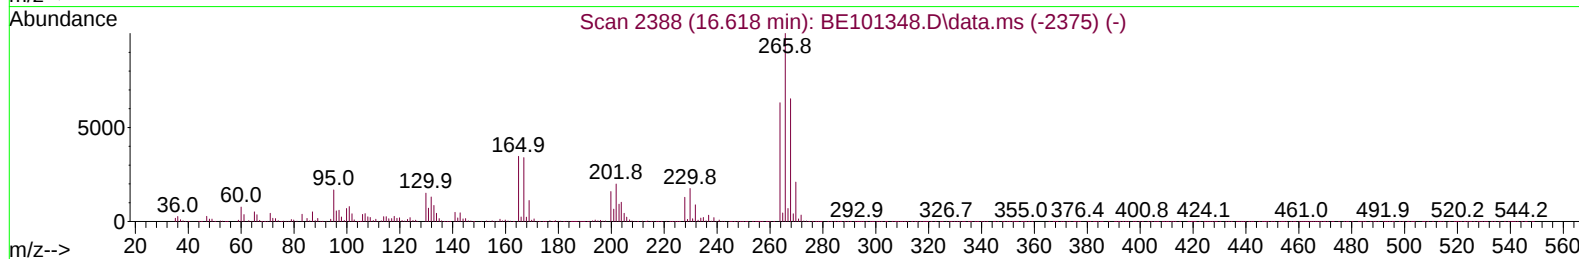
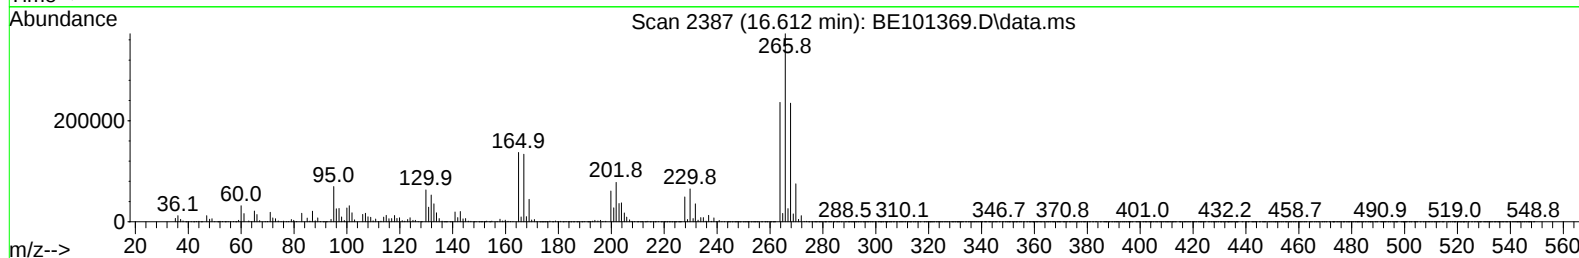


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091924\
Data File : BE101369.D
Acq On : 19 Sep 2024 8:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 03:09:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 17 16:03:42 2024
Response via : Initial Calibration

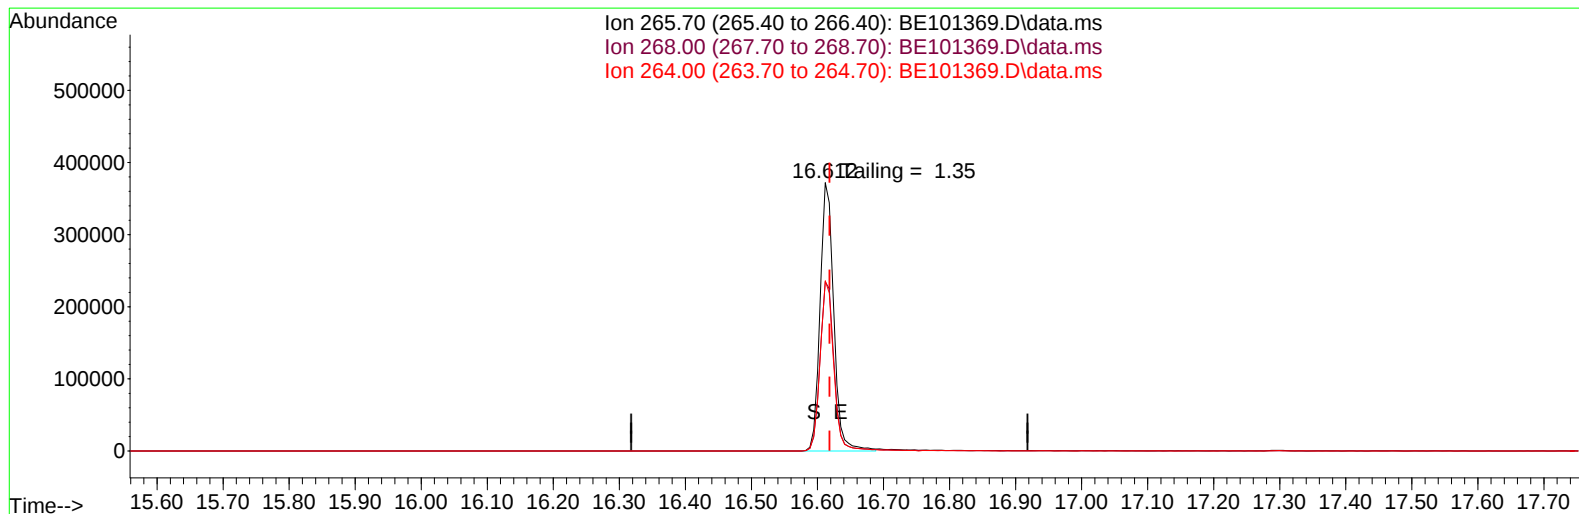

TIC: BE101369.D\data.ms

(70) Pentachlorophenol (C)




16.612min (-0.006) 39661.87 ng

response 542784

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.08
264.00	63.10	63.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091924\
Data File : BE101369.D
Acq On : 19 Sep 2024 8:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 03:09:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 17 16:03:42 2024
Response via : Initial Calibration

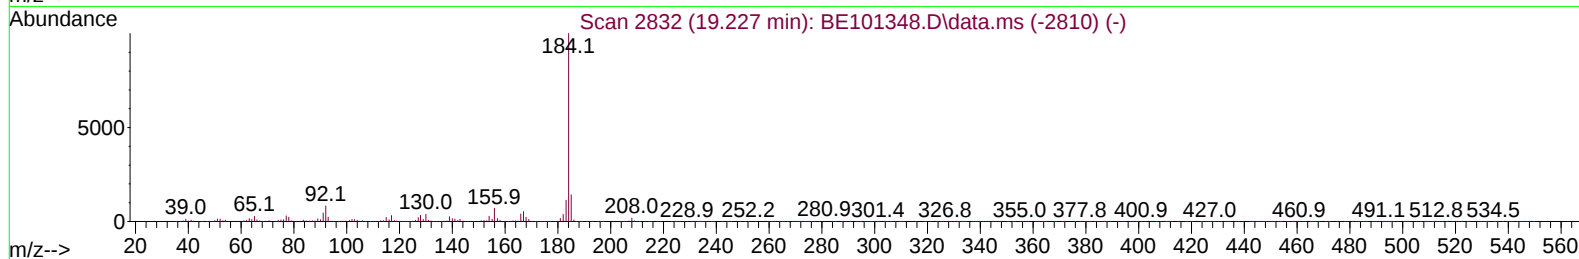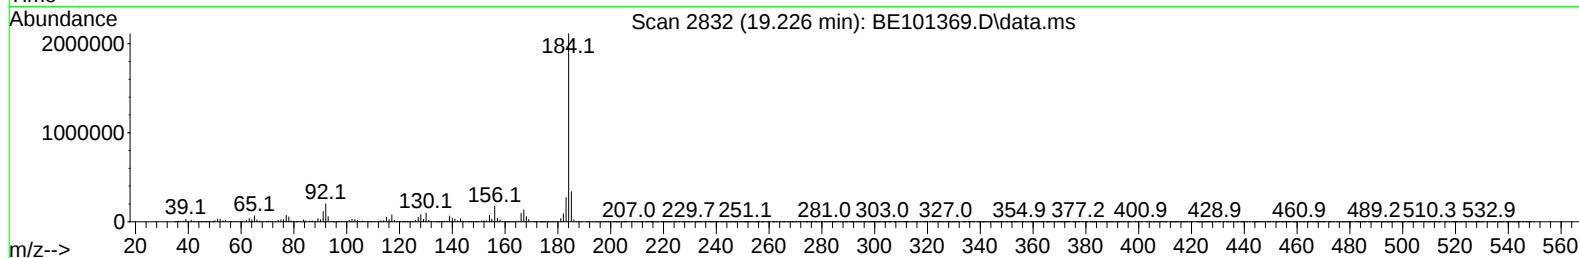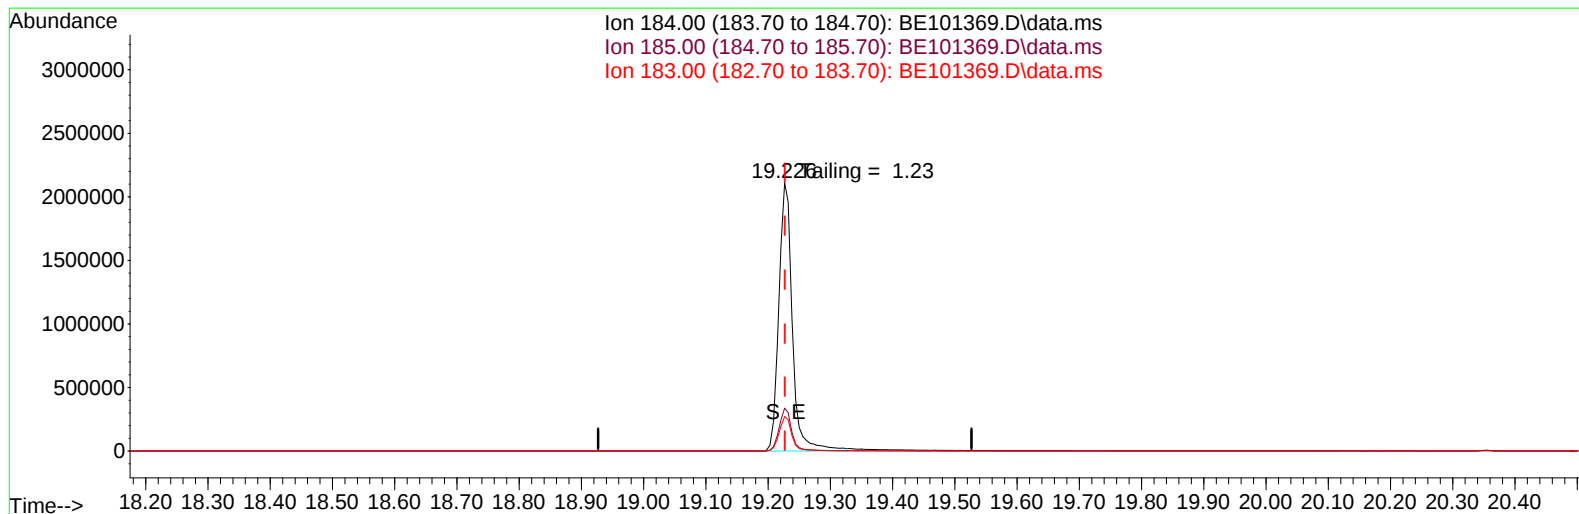

TIC: BE101369.D\data.ms

(77) Benzidine**19.226min (-0.000) 13752.63 ng****response 3269872**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	15.99
183.00	11.40	12.86
0.00	0.00	0.00