


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091924\
Data File : BE101369.D
Acq On : 19 Sep 2024 8:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 17 16:03:42 2024

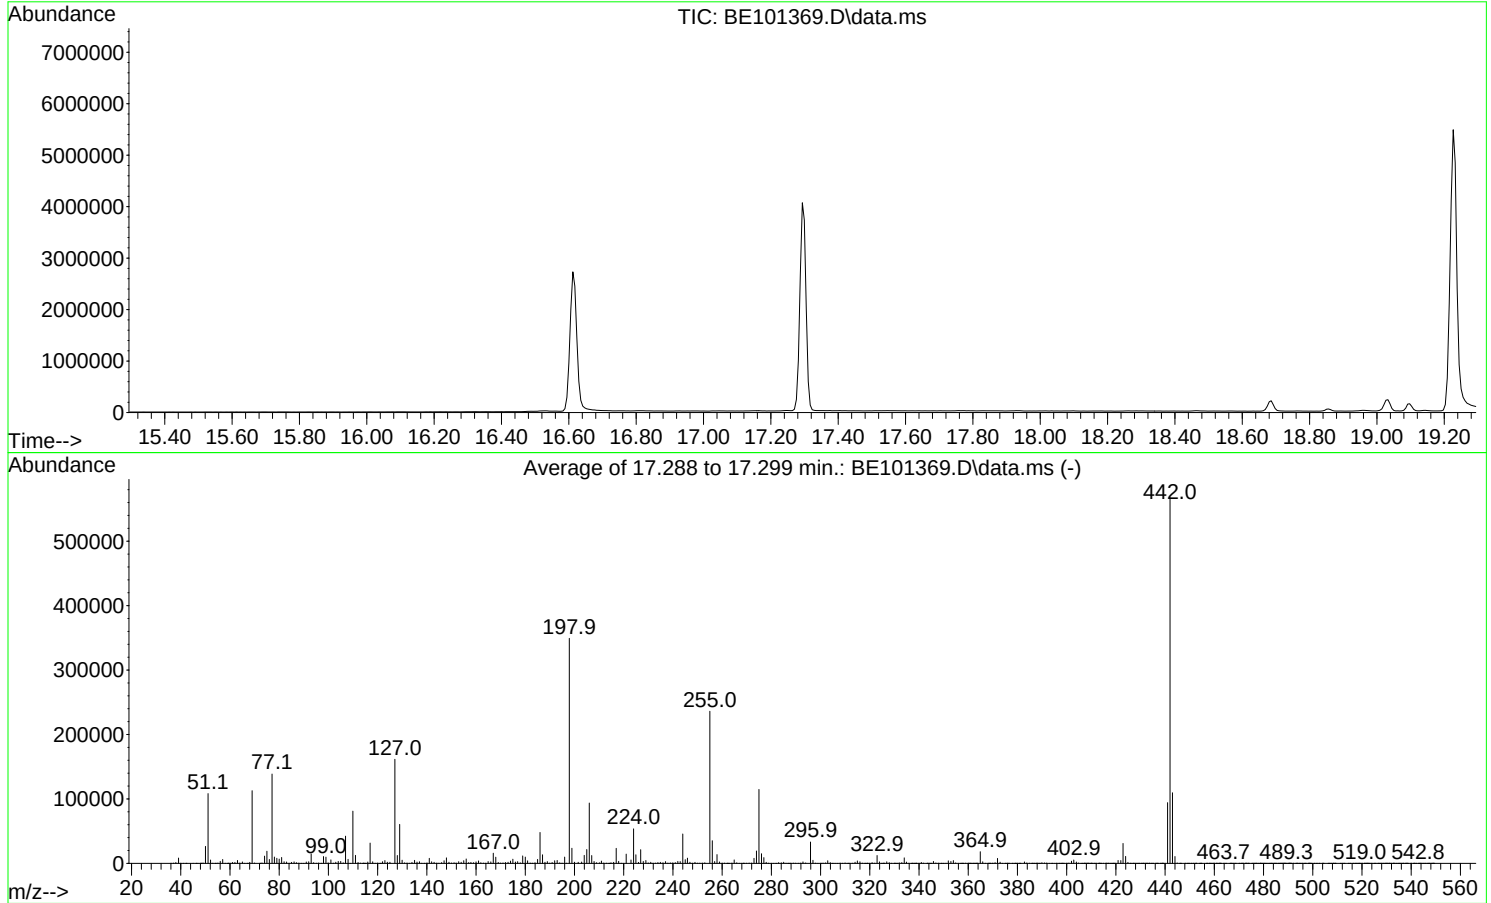




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	108296	PASS
68	69	0.00	2	1.4	1557	PASS
69	198	0.00	100	32.3	112800	PASS
70	69	0.00	2	0.5	587	PASS
127	198	10	80	46.2	161514	PASS
197	198	0.00	2	0.1	338	PASS
198	198	100	100	100.0	349269	PASS
199	198	5	9	6.7	23465	PASS
275	198	10	60	32.9	114765	PASS
365	198	1	100	5.2	18113	PASS
441	198	0.01	100	27.0	94221	PASS
442	442	50	100	100.0	567531	PASS
443	442	15	24	19.3	109630	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091924\
Data File : BE101369.D
Acq On : 19 Sep 2024 8:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Sep 20 03:09:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 17 16:03:42 2024
Response via : Initial Calibration

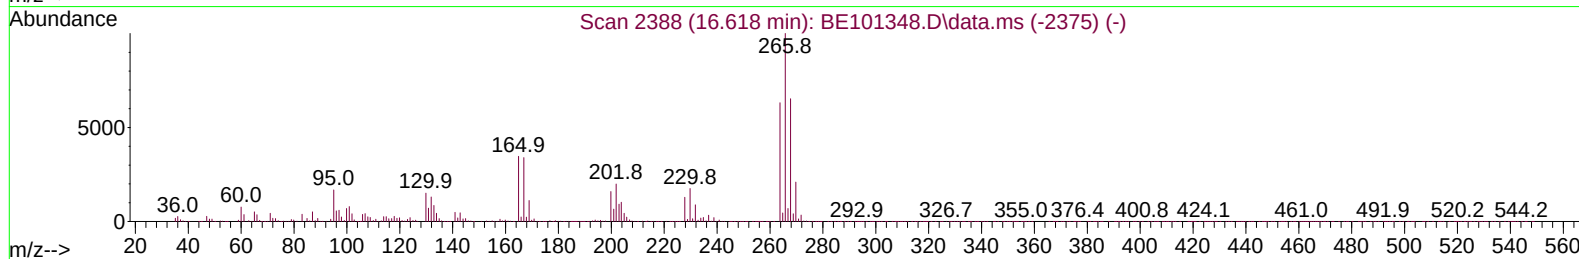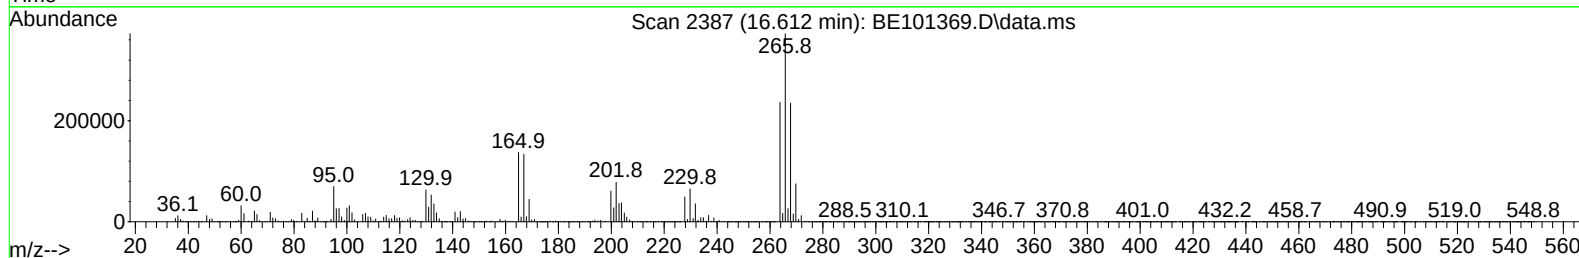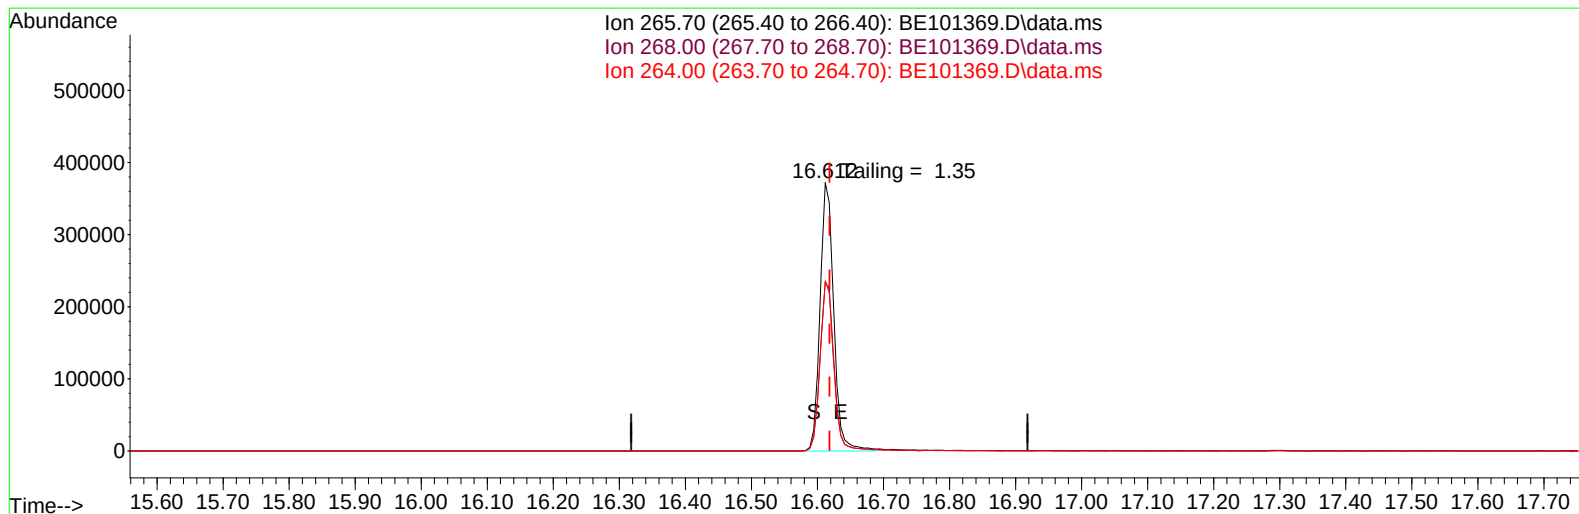

TIC: BE101369.D\data.ms

(70) Pentachlorophenol (C)

16.612min (-0.006) 39661.87 ng




response 542784

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.08
264.00	63.10	63.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE091924\
Data File : BE101369.D
Acq On : 19 Sep 2024 8:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Sep 20 03:09:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE091724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 17 16:03:42 2024
Response via : Initial Calibration

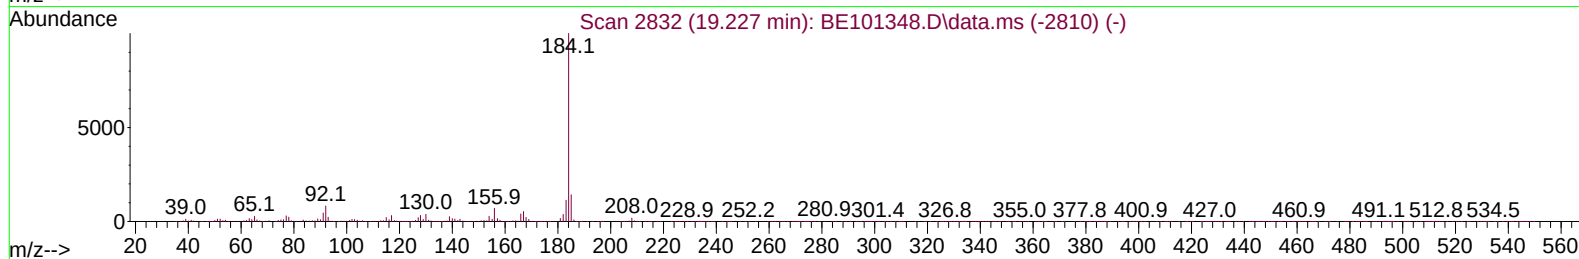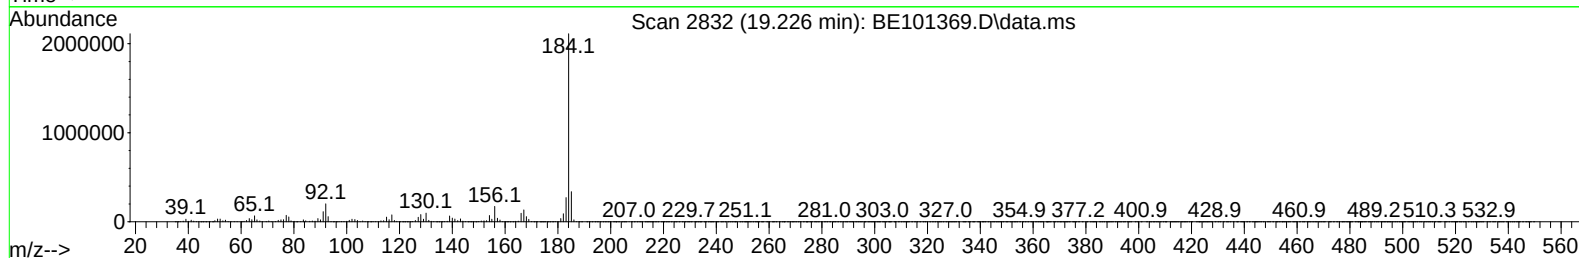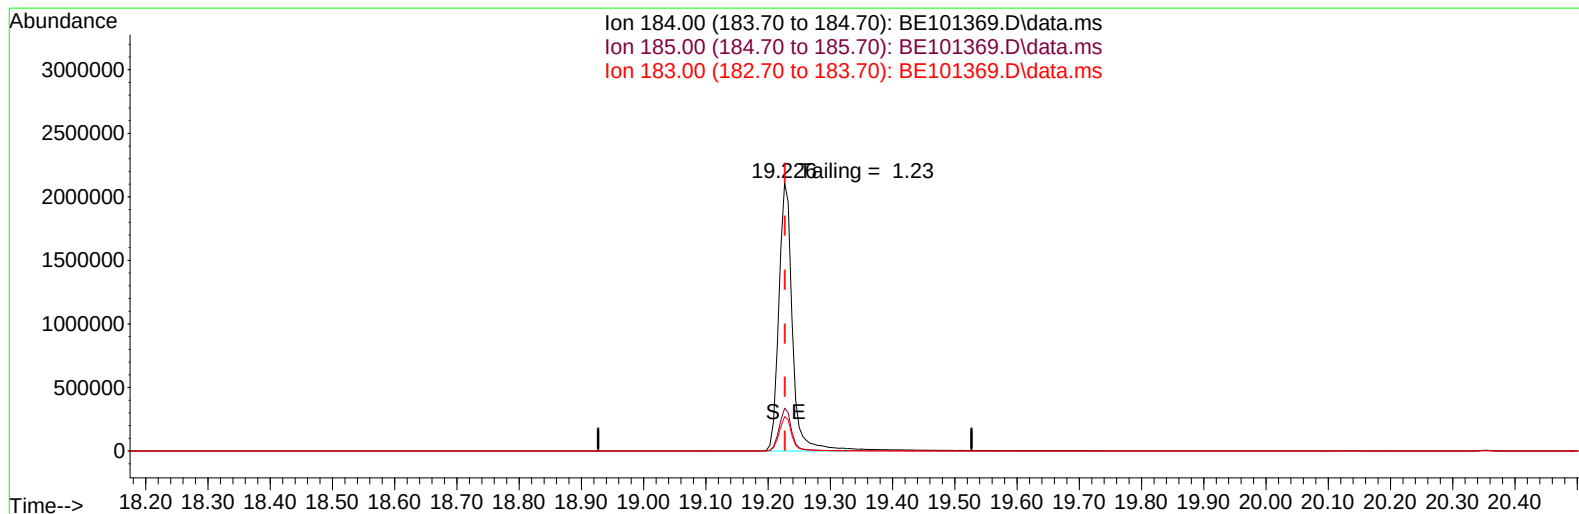

TIC: BE101369.D\data.ms

(77) Benzidine

19.226min (-0.000) 13752.63 ng

response 3269872

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	15.99
183.00	11.40	12.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2024	BNA_E	<u>BE101369.D</u>
Compound Name	Response	Retention Time
DDT	1724738	20.355
DDD	37413	19.92
DDE	1309	19.403
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38722	1763460	2.20

Instrument :
BNA_E
ClientSampleId :
DFTPP